
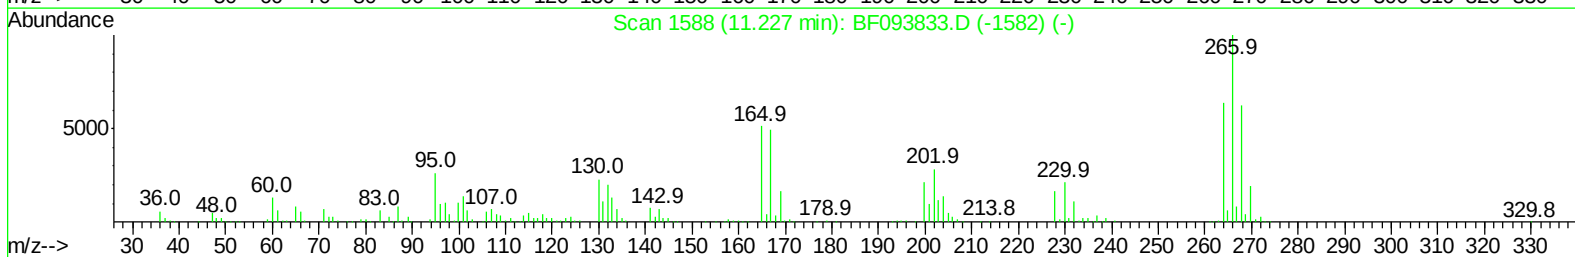
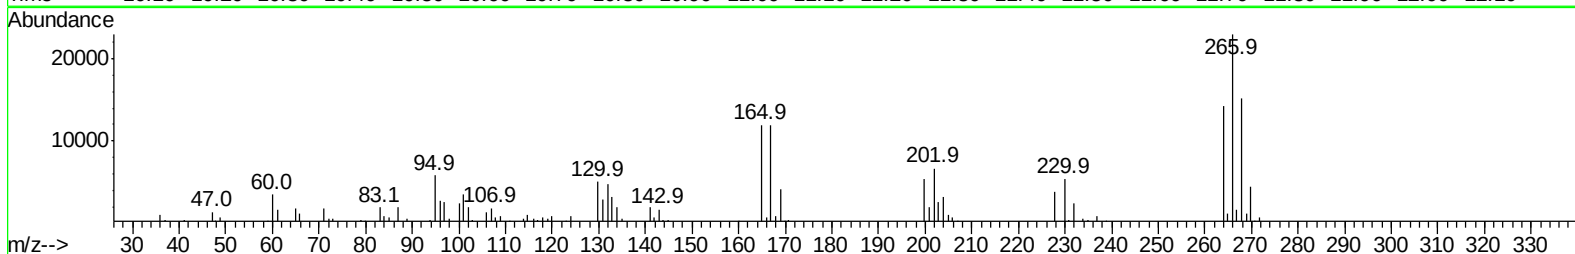


Data Path : Z:\HPCHEM1\BNA F\Data\BF040717\
Data File : BF094291.D
Acq On : 8 Apr 2017 1:06
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 07:23:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

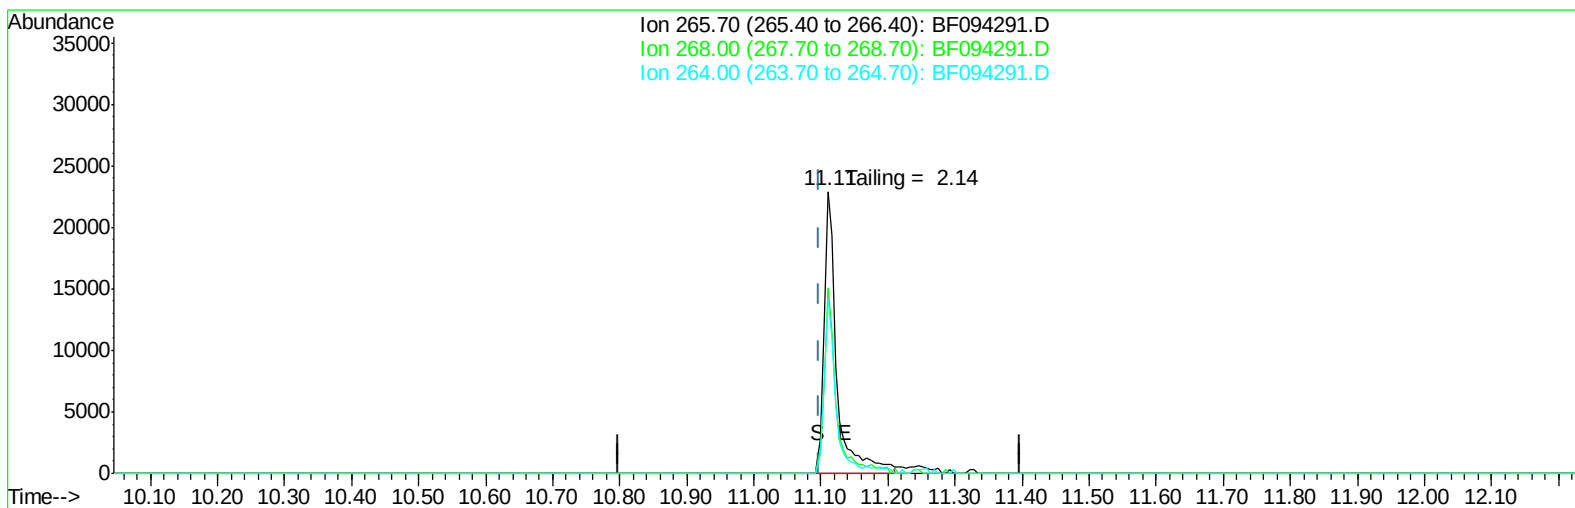

TIC: BF094291.D

(69) Pentachlorophenol (C)

11.110min (+0.012) 0.00ng

response 31319

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.07
264.00	64.60	61.86
0.00	0.00	0.00

