


Data Path : Z:\HPCHEM1\BNA F\Data\BF040717\
 Data File : BF094266.D
 Acq On : 7 Apr 2017 11:54
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 13:20:29 2017

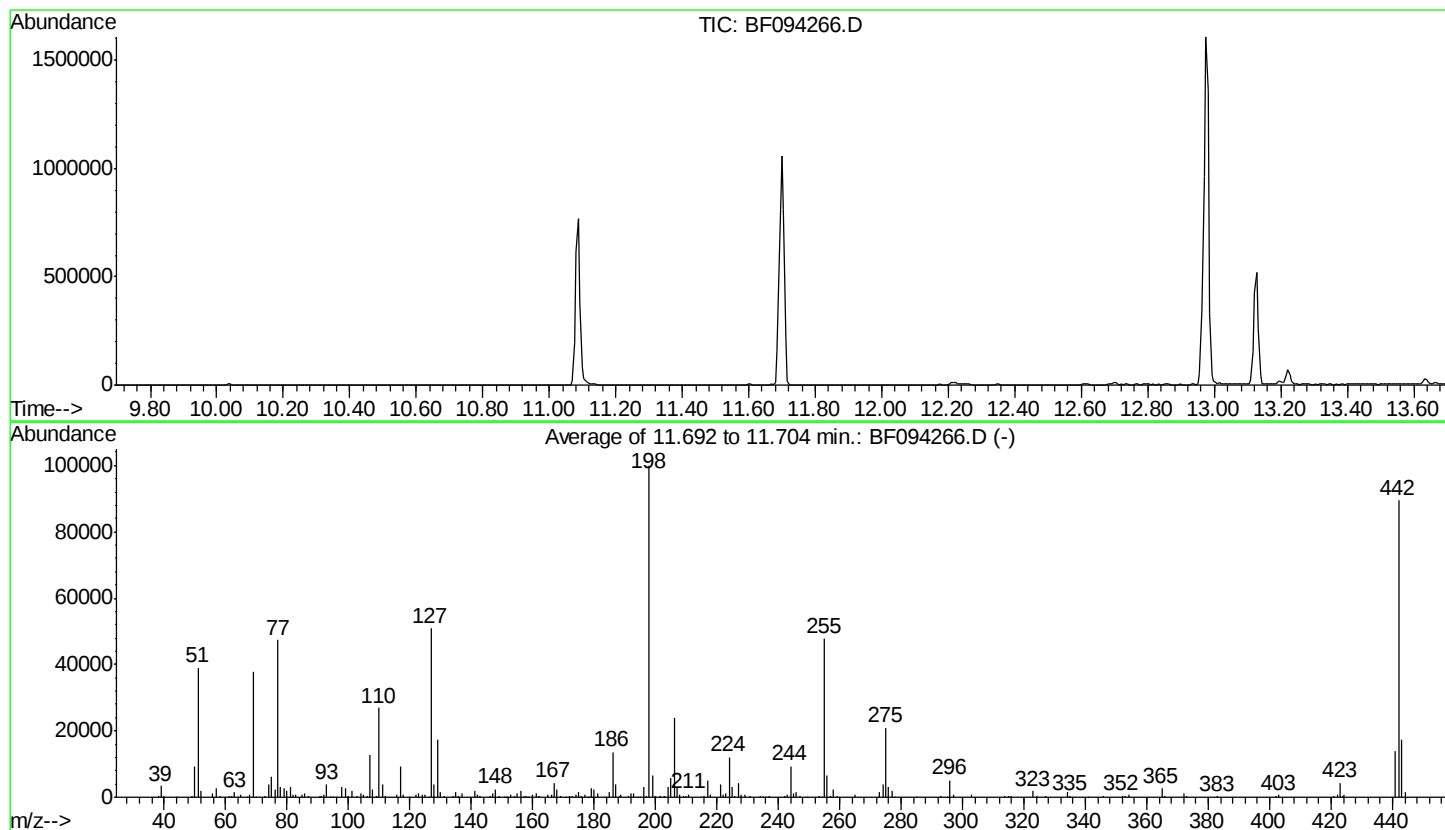

AutoFind: Scans 1667, 1668, 1669; Background Corrected with Scan 1662

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	39120	PASS
68	69	0.00	2	1.9	736	PASS
69	198	0.00	100	37.9	37872	PASS
70	69	0.00	2	0.3	111	PASS
127	198	10	80	50.8	50762	PASS
197	198	0.00	2	0.4	366	PASS
198	198	100	100	100.0	99941	PASS
199	198	5	9	6.7	6692	PASS
275	198	10	60	20.9	20904	PASS
365	198	1	100	2.6	2626	PASS
441	442	0.01	24	15.5	13881	PASS
442	198	50	100	89.5	89453	PASS
443	442	15	24	19.3	17254	PASS