


Data Path : Z:\HPCHEM1\BNA_F\Data\BF040717\
 Data File : BF094291.D
 Acq On : 8 Apr 2017 1:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 13:20:29 2017

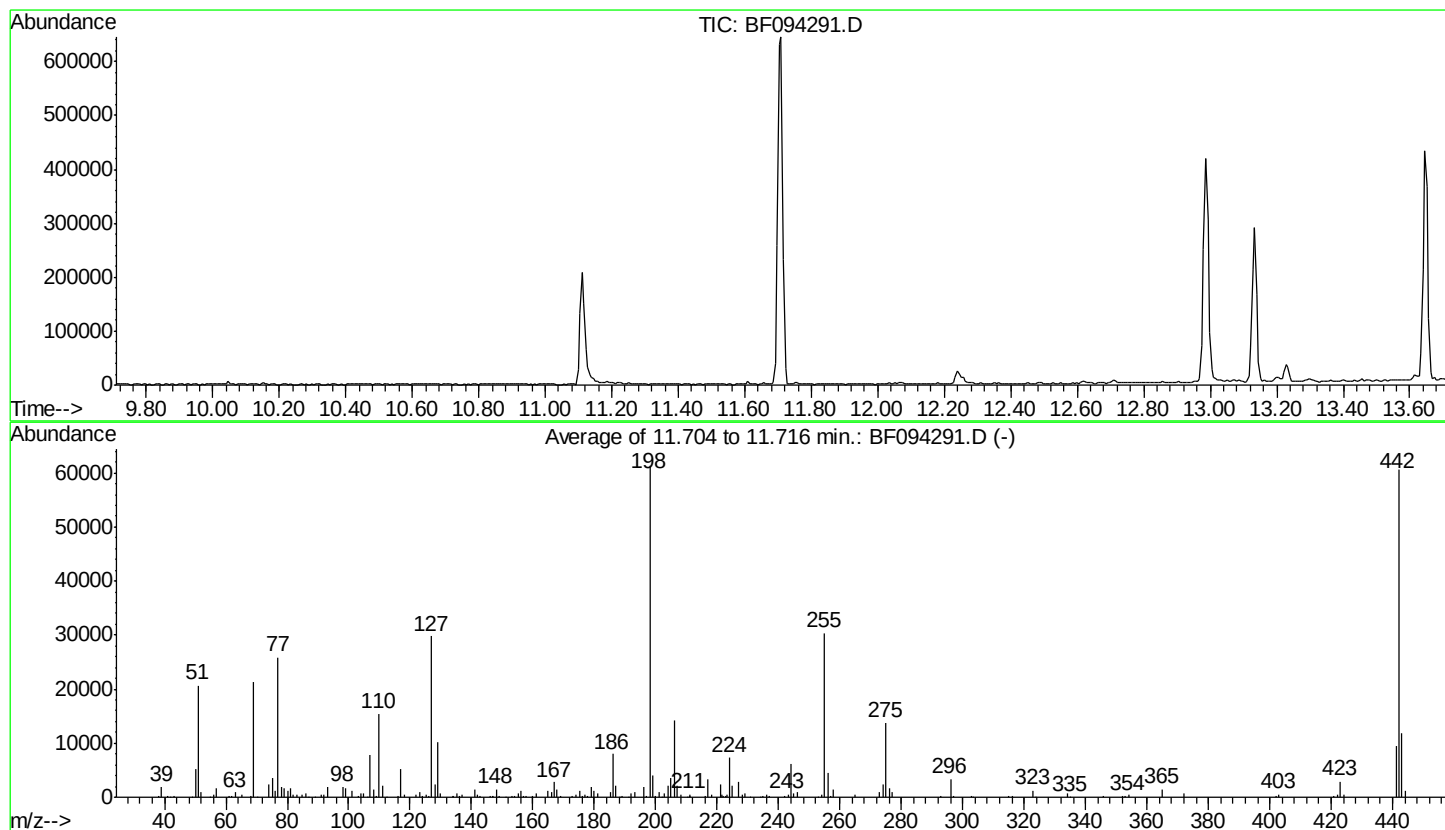

AutoFind: Scans 1669, 1670, 1671; Background Corrected with Scan 1663

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	20643	PASS
68	69	0.00	2	1.5	316	PASS
69	198	0.00	100	34.6	21253	PASS
70	69	0.00	2	0.5	112	PASS
127	198	10	80	48.6	29842	PASS
197	198	0.00	2	0.3	176	PASS
198	198	100	100	100.0	61357	PASS
199	198	5	9	6.4	3920	PASS
275	198	10	60	22.6	13855	PASS
365	198	1	100	2.5	1534	PASS
441	442	0.01	24	15.6	9474	PASS
442	198	50	100	99.0	60730	PASS
443	442	15	24	19.3	11741	PASS