


Data Path : Z:\HPCHEM1\BNA_F\Data\BF040815\
 Data File : BF078339.D
 Acq On : 8 Apr 2015 15:21
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 14:42:25 2015

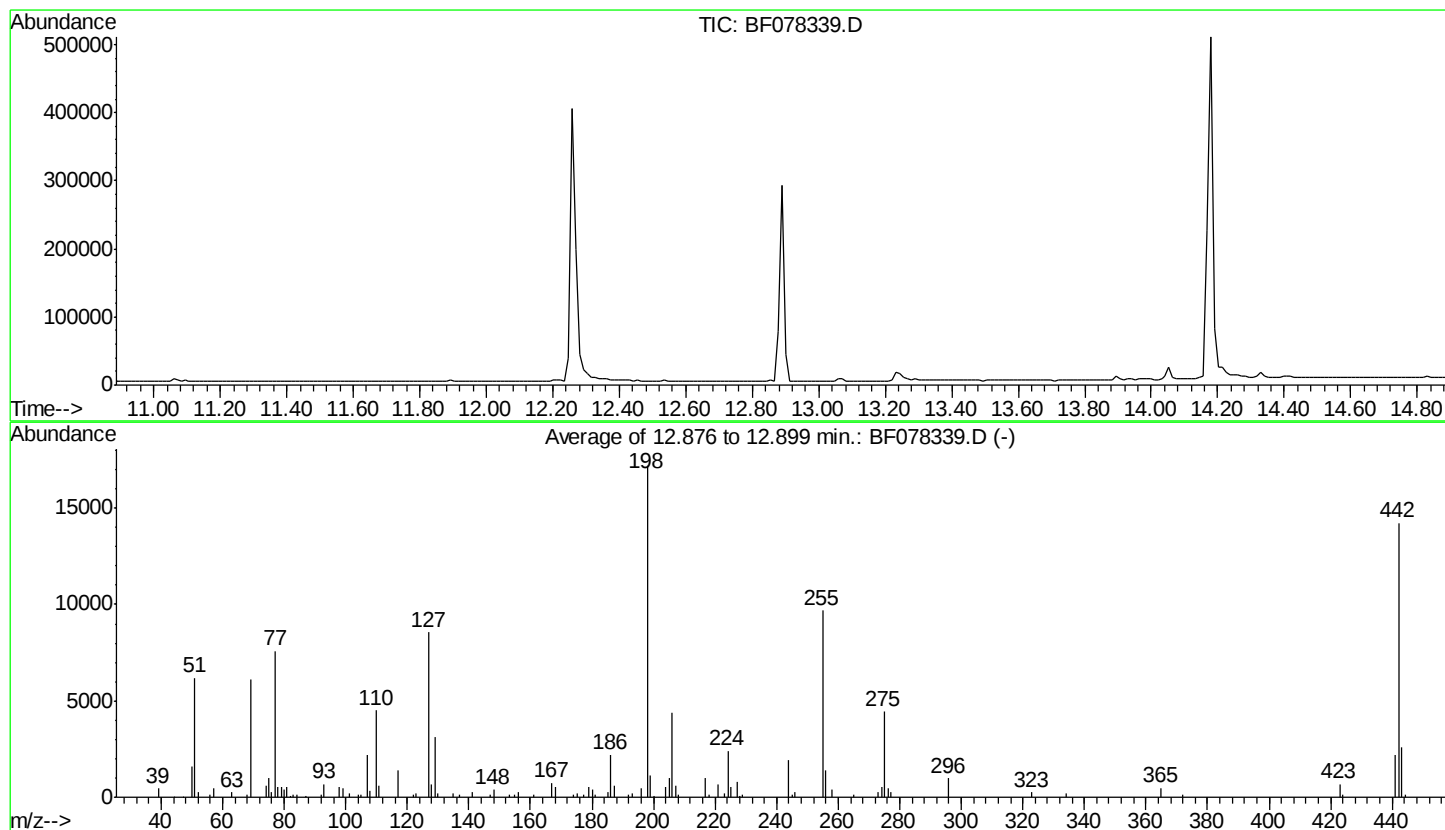

AutoFind: Scans 1049, 1050, 1051; Background Corrected with Scan 1046

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	6180	PASS
68	69	0.00	2	1.7	104	PASS
69	198	0.00	100	35.6	6120	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	8565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17207	PASS
199	198	5	9	6.4	1105	PASS
275	198	10	60	25.8	4443	PASS
365	198	1	100	2.7	466	PASS
441	442	0.01	24	15.5	2202	PASS
442	198	50	100	82.8	14239	PASS
443	442	15	24	18.3	2603	PASS