
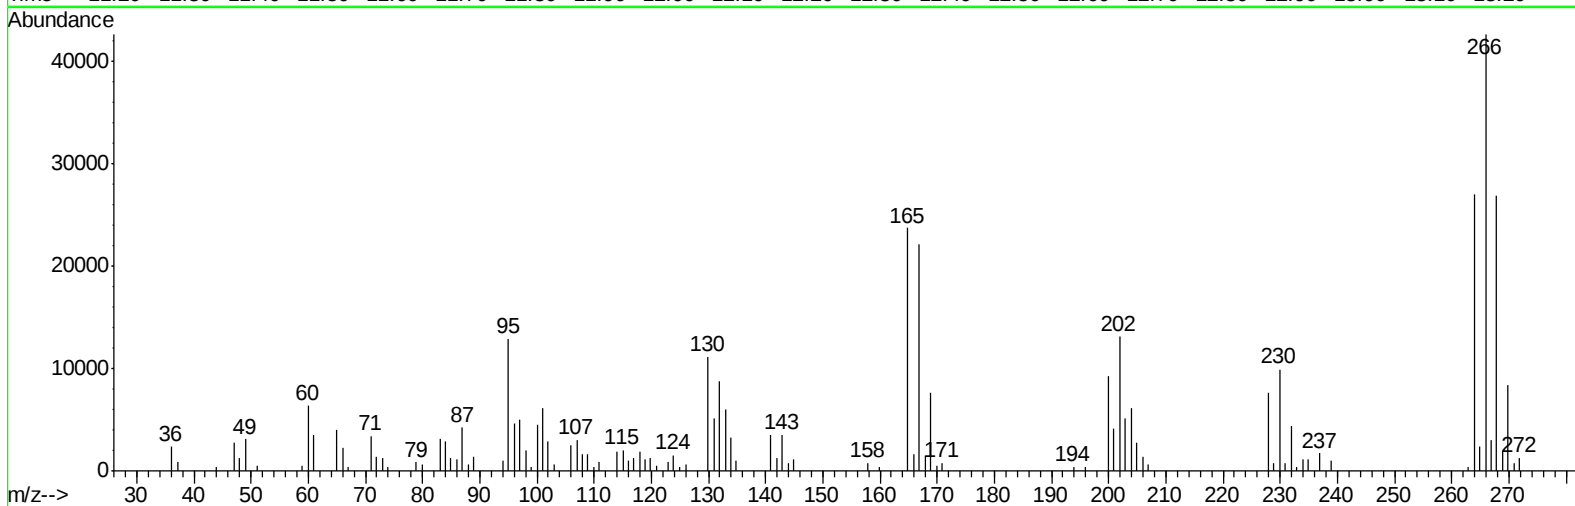


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040815\
Data File : BF078339.D
Acq On : 8 Apr 2015 15:21
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 07:59:30 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 09 00:49:15 2015
Response via : Initial Calibration

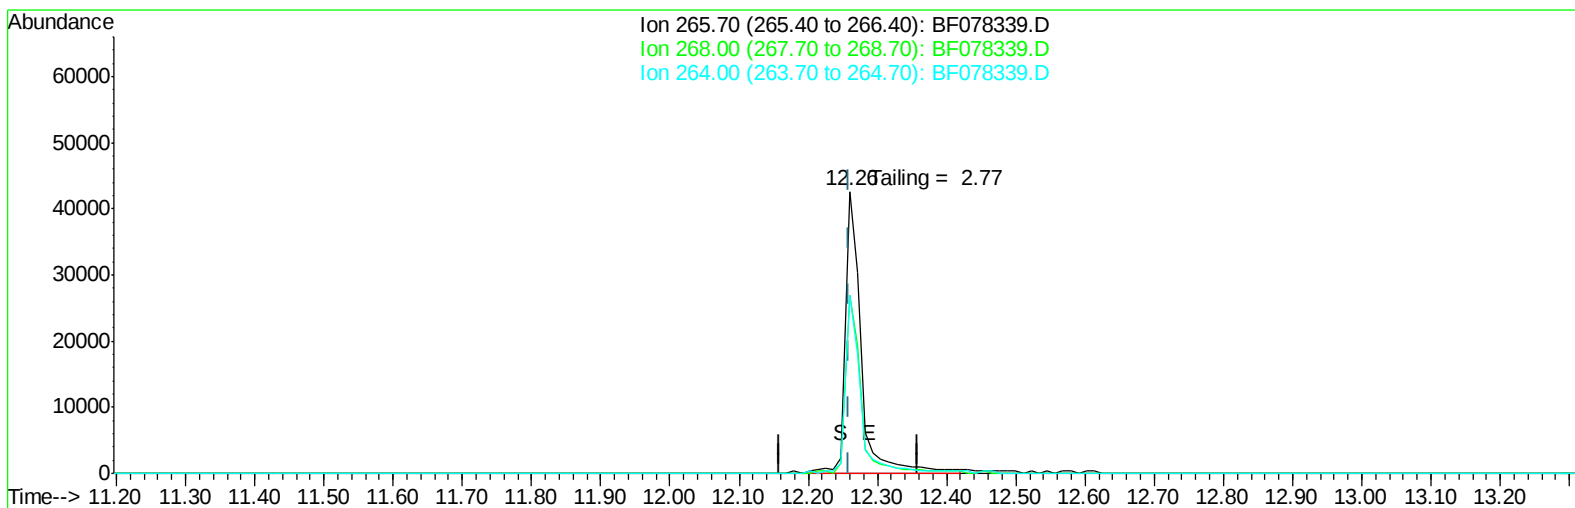

TIC: BF078339.D

(69) Pentachlorophenol (C)



12.259min (-0.000) 0.00ng

response 62222

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	63.10
264.00	62.50	63.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040815\
Data File : BF078339.D
Acq On : 8 Apr 2015 15:21
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 07:59:30 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 09 00:49:15 2015
Response via : Initial Calibration

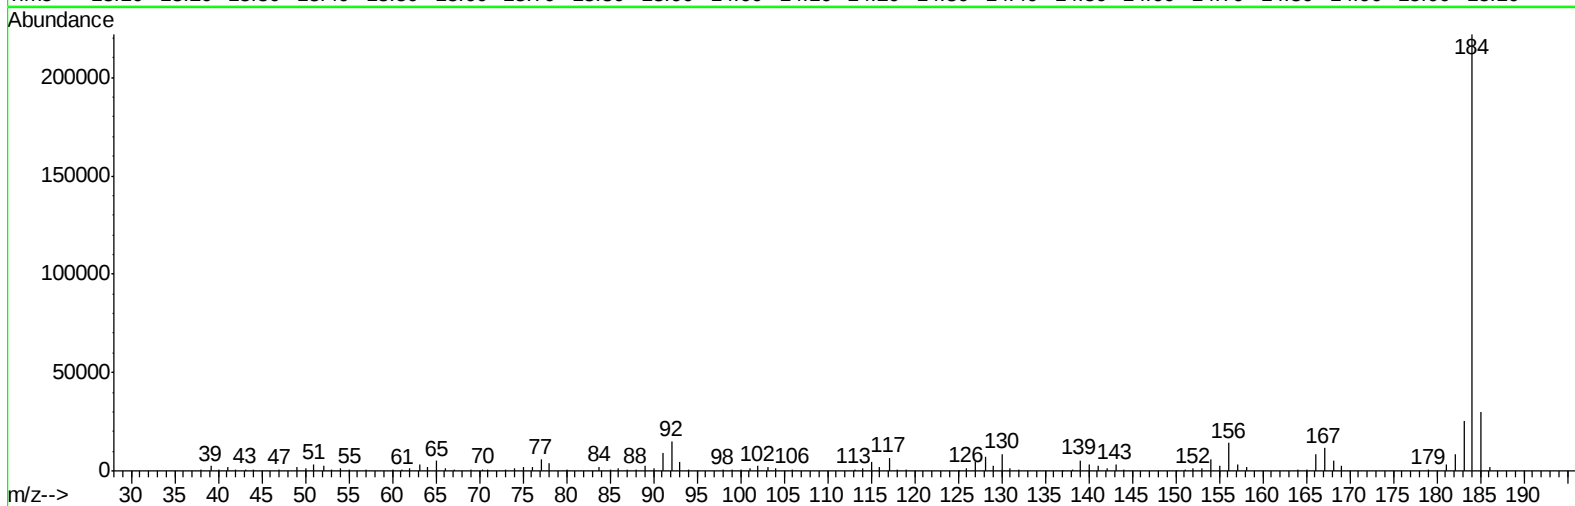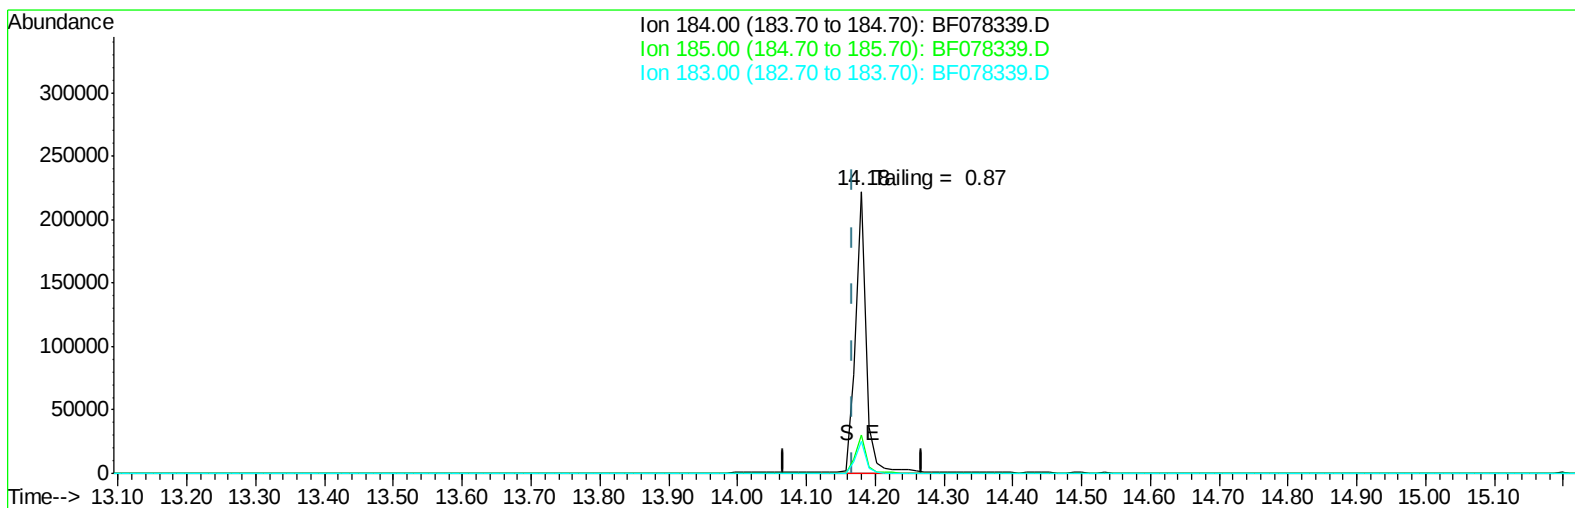

TIC: BF078339.D

(76) Benzidine

14.179min (+0.011) 0.00ng

response 240354

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.47
183.00	11.90	11.38
0.00	0.00	0.00