

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
 Data File : BF086173.D
 Acq On : 8 Apr 2016 17:34
 Operator : UM/SJ
 Sample : H2343-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-2

Quant Time: Apr 08 23:20:38 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 01 23:17:06 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	123326	20.00	ng	-0.05
21) Naphthalene-d8	8.01	136	495075	20.00	ng	-0.06
38) Acenaphthene-d10	9.77	164	240195	20.00	ng	-0.05
63) Phenanthrene-d10	11.24	188	458152	20.00	ng	-0.06
75) Chrysene-d12	13.88	240	348421	20.00	ng	-0.05
86) Perylene-d12	15.28	264	248399	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	514515	71.31	ng	-0.05
7) Phenol-d6	6.37	99	438010	47.79	ng	-0.05
23) Nitrobenzene-d5	7.30	82	777145	92.57	ng	-0.05
41) 2,4,6-Tribromophenol	10.56	330	323592	143.53	ng	-0.05
44) 2-Fluorobiphenyl	9.09	172	1389679	96.20	ng	-0.05
78) Terphenyl-d14	12.83	244	1200481	80.99	ng	-0.05
Target Compounds						
9) Benzaldehyde	6.50	77	18504	3.75	ng	Qvalue 89
15) Benzyl Alcohol	6.88	79	11954	2.02	ng	# 51
19) n-Nitroso-di-n-propylamine	7.30	70	102059	17.97	ng	# 78
25) Isophorone	7.30	82	776608	46.86	ng	# 68
50) 2,6-Dinitrotoluene	9.77	165	29328	7.79	ng	# 18
56) 2,4-Dinitrotoluene	9.77	165	29328	6.16	ng	# 36
66) 4-Bromophenyl-phenylether	10.56	248	21671	4.63	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
Data File : BF086173.D
Acq On : 8 Apr 2016 17:34
Operator : UM/SJ
Sample : H2343-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Time: Apr 08 23:20:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

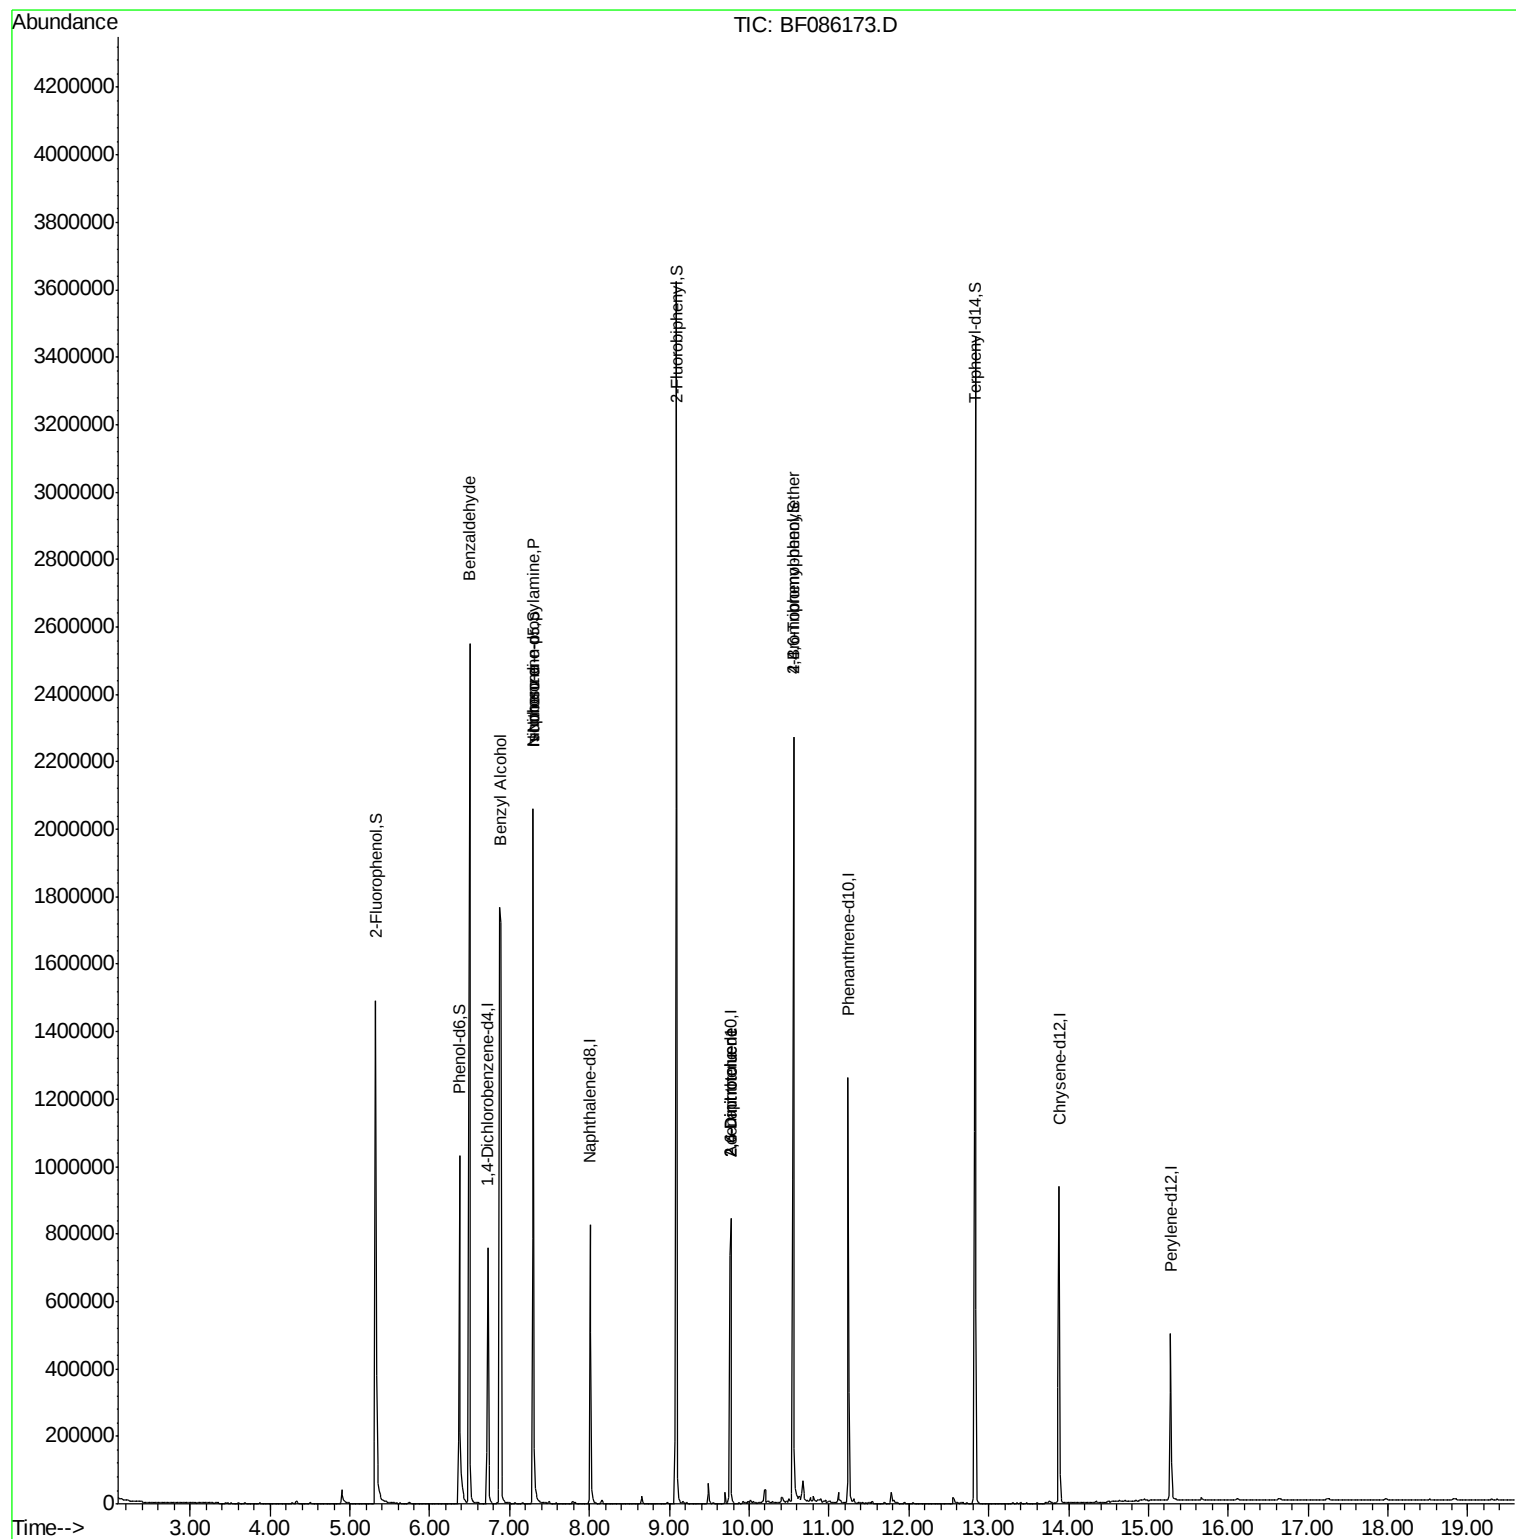

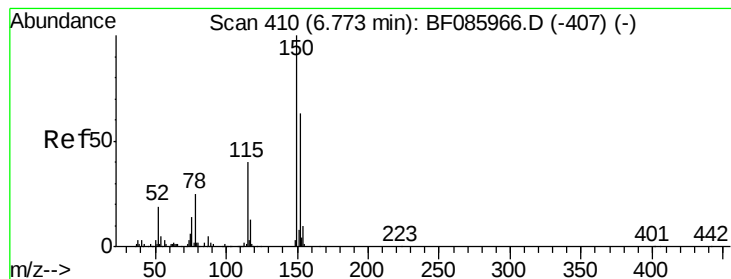

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.73 min Scan# 406

Delta R.T. -0.05 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34

Instrument :

BNA_F

ClientSampleId :

MW-2


Tgt Ion:152 Resp: 123326

Ion Ratio Lower Upper

152 100

150 155.7 124.2 186.2




115 60.3 47.0 70.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

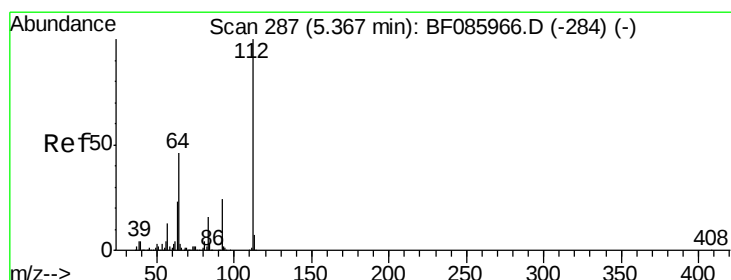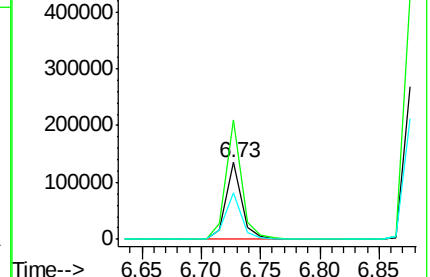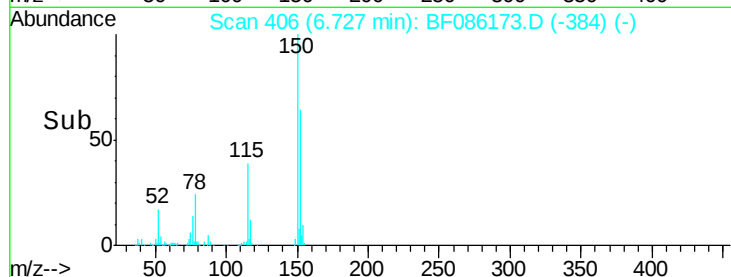

#5

2-Fluorophenol

Concen: 71.31 ng

RT: 5.32 min Scan# 283

Delta R.T. -0.05 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34


Tgt Ion:112 Resp: 514515

Ion Ratio Lower Upper

112 100

64 52.8 39.9 59.9



63 26.7 20.2 30.2



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

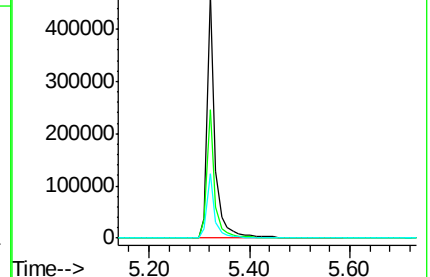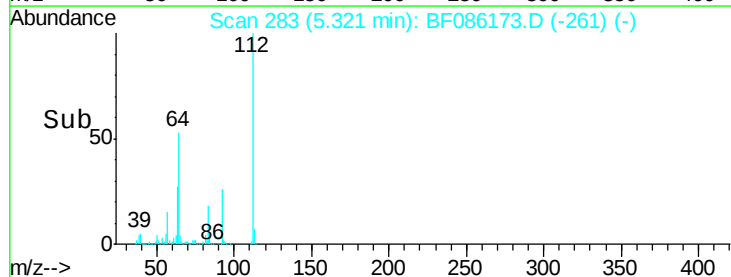



#7

Phenol-d6

Concen: 47.79 ng

RT: 6.37 min Scan# 375

Delta R.T. -0.05 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34

Instrument :

BNA_F

ClientSampleId :

MW-2


Tgt Ion: 99 Resp: 438010

Ion Ratio Lower Upper

99 100

42 13.6 11.1 16.7




71 30.3 24.9 37.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

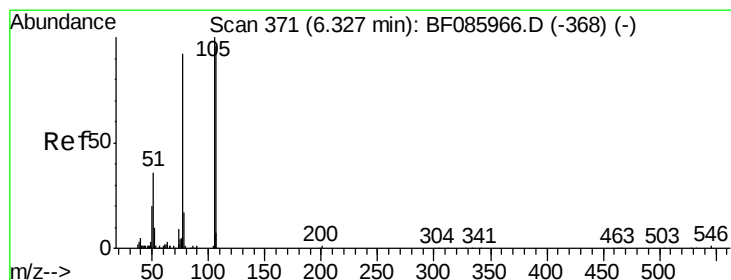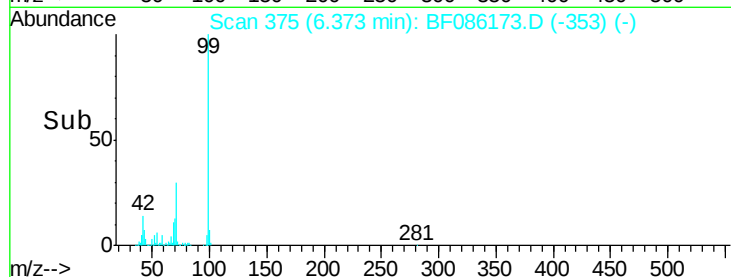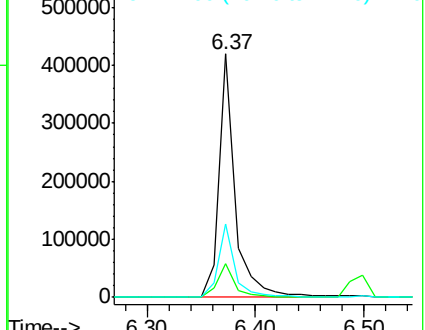

#9

Benzaldehyde

Concen: 3.75 ng

RT: 6.50 min Scan# 386

Delta R.T. 0.17 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34


Tgt Ion: 77 Resp: 18504

Ion Ratio Lower Upper

77 100

105 87.3 80.1 120.1



106 85.9 75.0 115.0

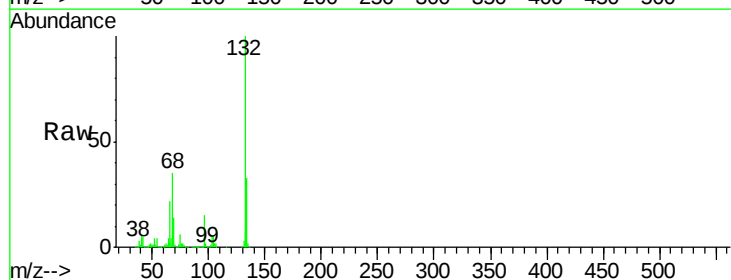


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



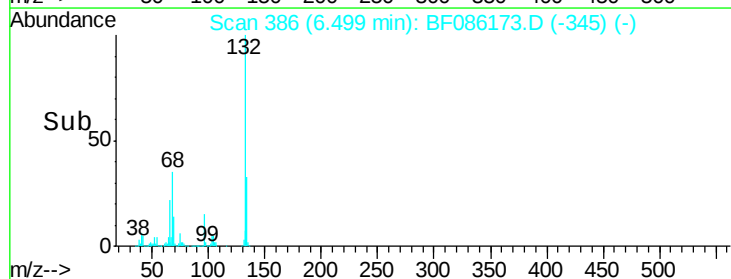
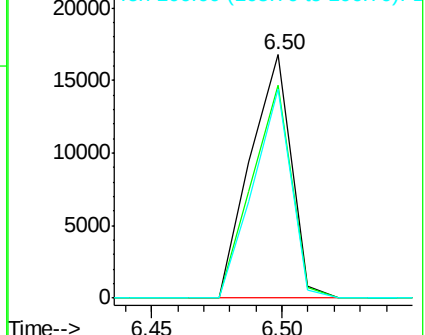


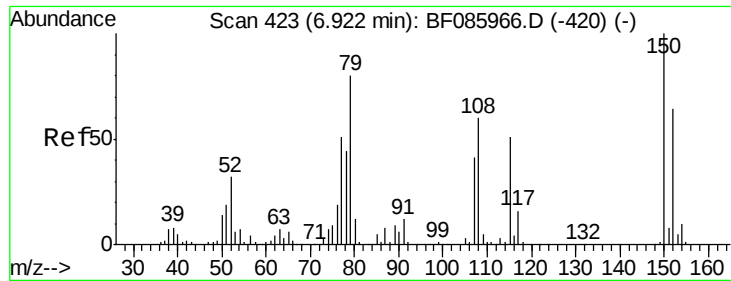

#15
Benzyl Alcohol
Concen: 2.02 ng
RT: 6.88 min Scan# 419
Delta R.T. -0.05 min
Lab File: BF086173.D
Acq: 8 Apr 2016 17:34




Instrument :
BNA_F
ClientSampleId :
MW-2


Tgt Ion: 79 Resp: 11954
Ion Ratio Lower Upper
79 100
108 30.1 61.8 92.6#
77 95.3 49.6 74.4#

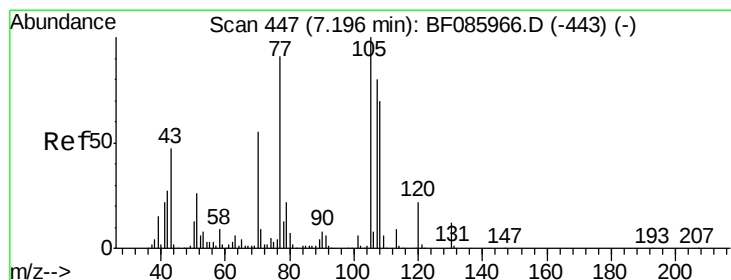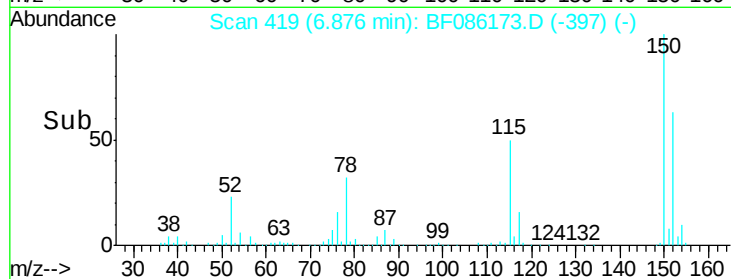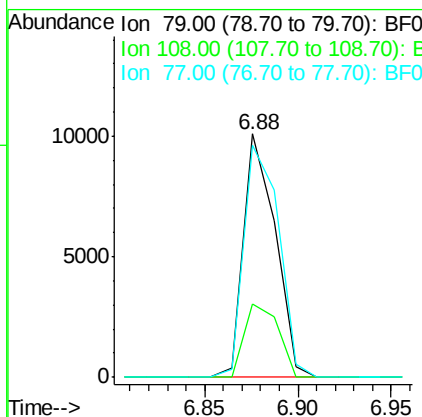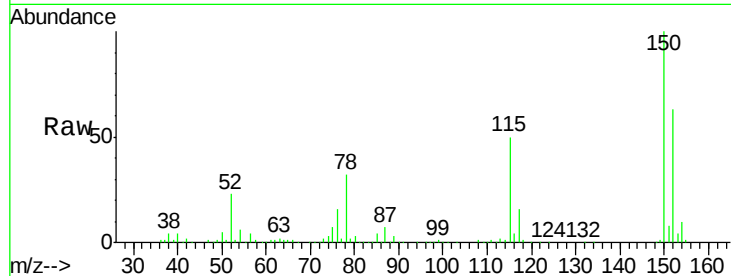

#19
n-Nitroso-di-n-propylamine
Concen: 17.97 ng
RT: 7.30 min Scan# 456
Delta R.T. 0.10 min
Lab File: BF086173.D
Acq: 8 Apr 2016 17:34

Tgt Ion: 70 Resp: 102059
Ion Ratio Lower Upper
70 100
42 40.4 37.1 55.7
101 0.0 8.6 12.8#
130 2.3 19.6 29.4#


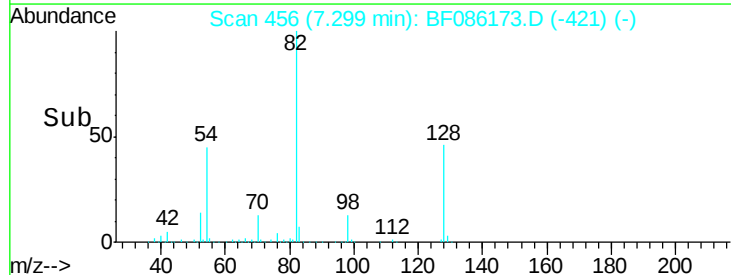
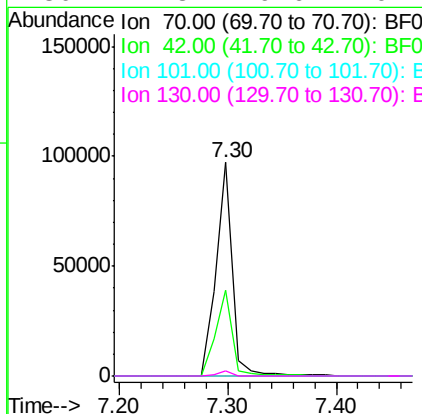
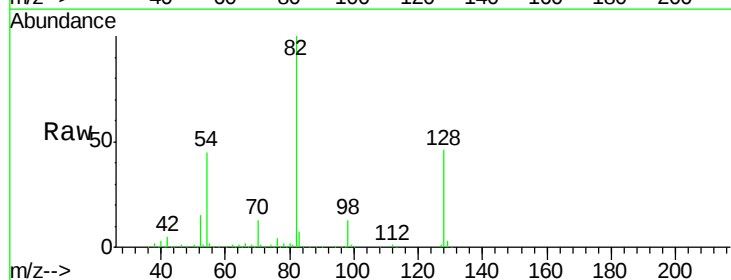


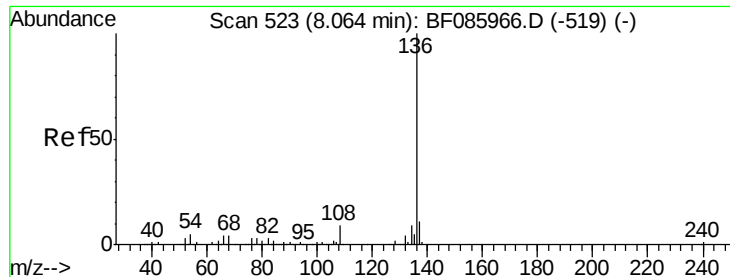

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.01 min Scan# 518
Delta R.T. -0.06 min
Lab File: BF086173.D
Acq: 8 Apr 2016 17:34




Instrument :
BNA_F
ClientSampleId :
MW-2


Tgt Ion:	136	Resp:	495075
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.1	13.7
54	8.7	7.4	11.0
68	7.0	5.8	8.8

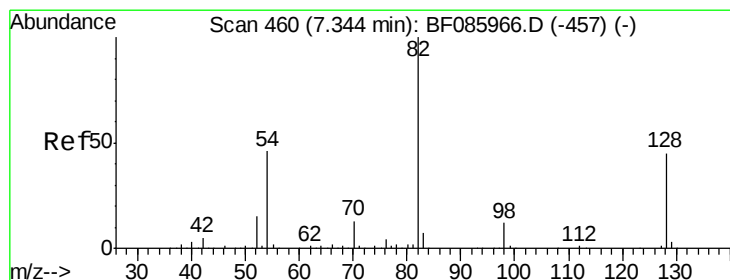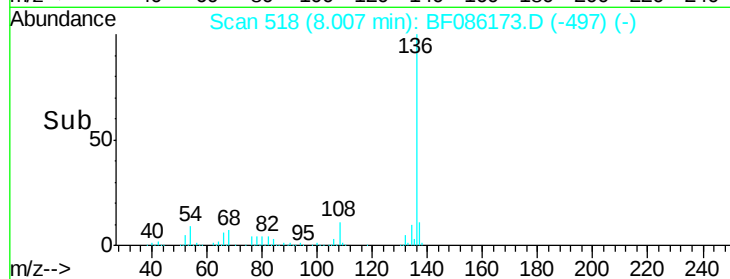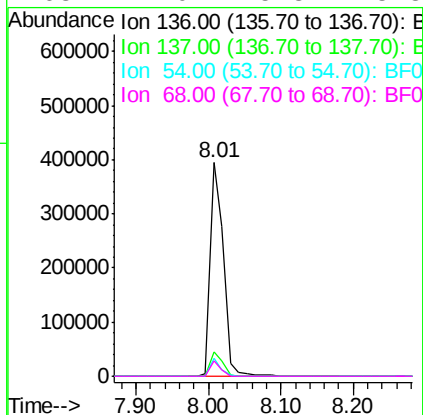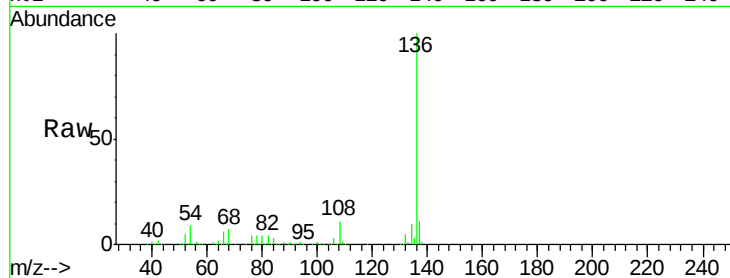

#23
Nitrobenzene-d5
Concen: 92.57 ng
RT: 7.30 min Scan# 456
Delta R.T. -0.05 min
Lab File: BF086173.D
Acq: 8 Apr 2016 17:34

Tgt Ion:	82	Resp:	777145
Ion	Ratio	Lower	Upper
82	100		
128	46.3	41.8	62.8
54	44.9	33.4	50.0

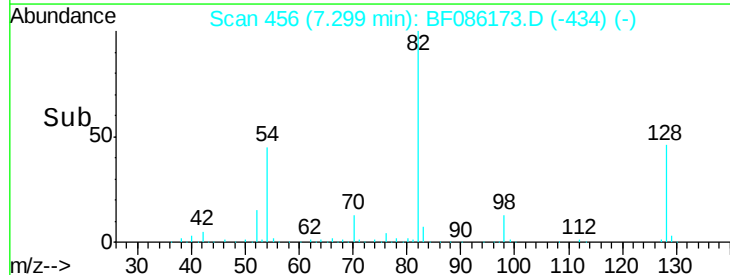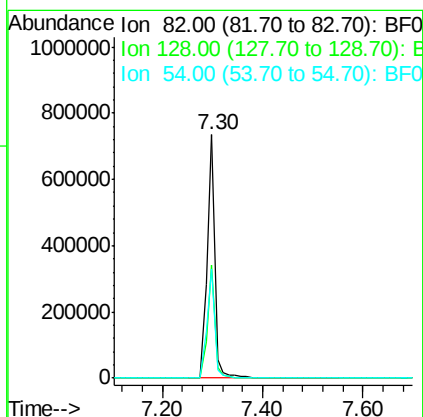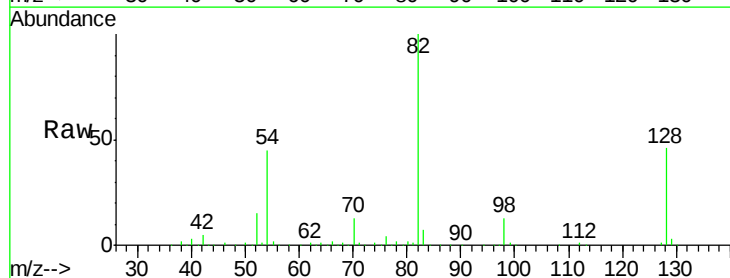

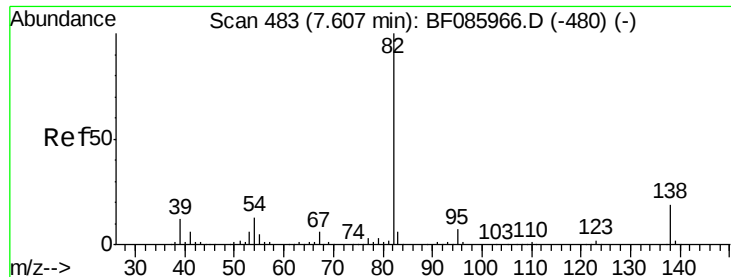

#25

Isophorone

Concen: 46.86 ng

RT: 7.30 min Scan# 456

Delta R.T. -0.31 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34

Instrument :

BNA_F

ClientSampleId :

MW-2


Tgt Ion: 82 Resp: 776608

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#




138 0.0 12.9 19.3#



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0

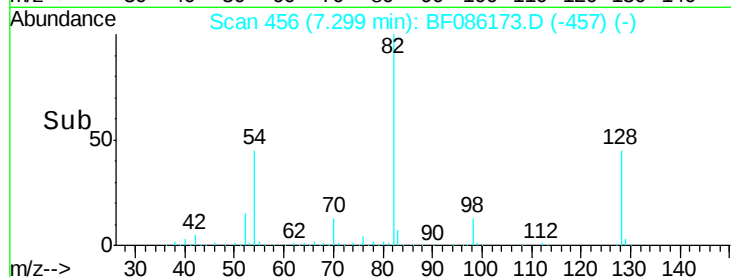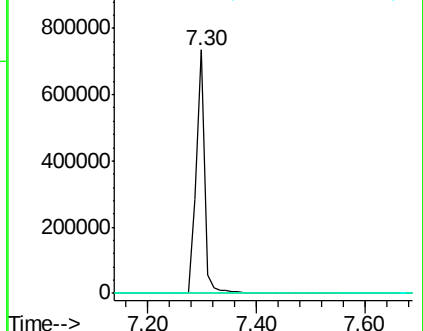

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.77 min Scan# 672

Delta R.T. -0.05 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34


Tgt Ion: 164 Resp: 240195

Ion Ratio Lower Upper

164 100

162 105.7 82.1 123.1



160 50.5 37.4 56.2




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

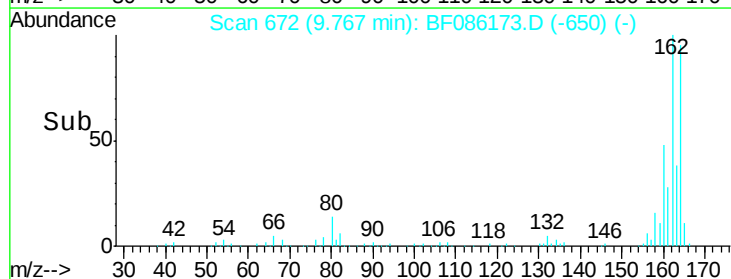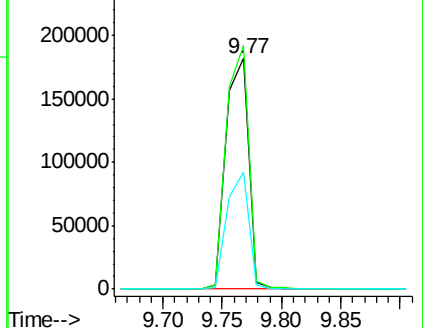


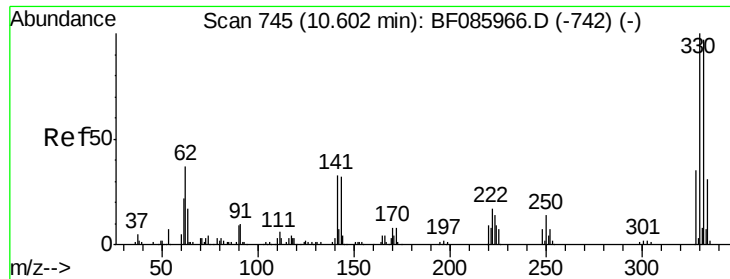




#41
 2,4,6-Tribromophenol
 Concen: 143.53 ng
 RT: 10.56 min Scan# 741
 Delta R.T. -0.05 min
 Lab File: BF086173.D
 Acq: 8 Apr 2016 17:34

Instrument :
 BNA_F
 ClientSampleId :
 MW-2

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.4	78.2	117.2
141	34.4	31.5	47.3

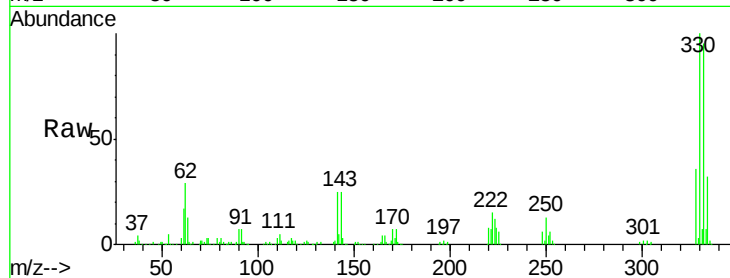


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

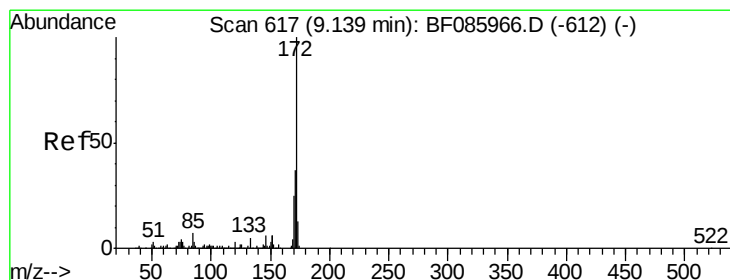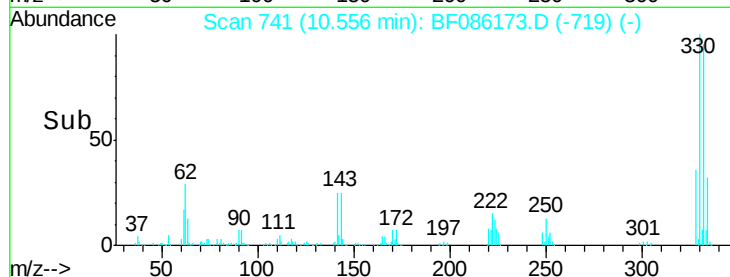
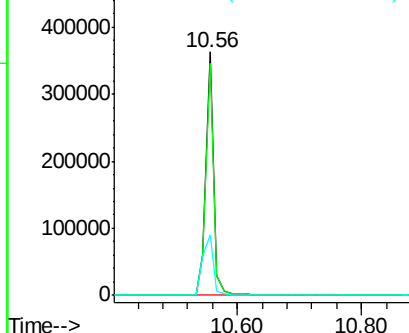



#44
 2-Fluorobiphenyl
 Concen: 96.20 ng
 RT: 9.09 min Scan# 613
 Delta R.T. -0.05 min
 Lab File: BF086173.D
 Acq: 8 Apr 2016 17:34

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.4	44.2
170	24.9	19.8	29.6

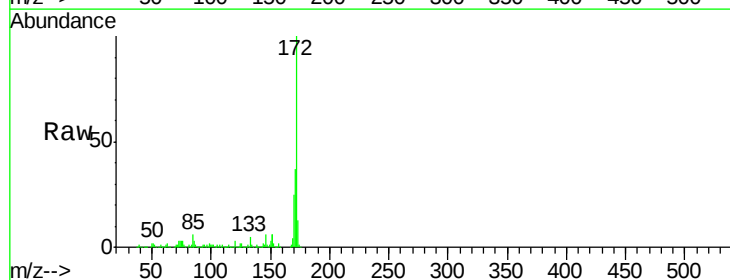

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

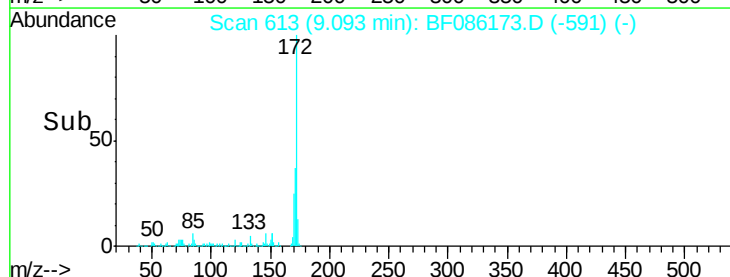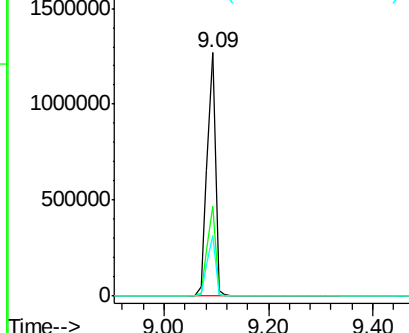


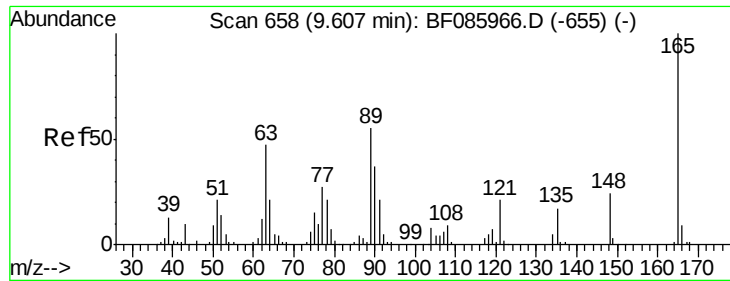




#50
 2,6-Dinitrotoluene
 Concen: 7.79 ng
 RT: 9.77 min Scan# 672
 Delta R.T. 0.16 min
 Lab File: BF086173.D
 Acq: 8 Apr 2016 17:34

Instrument :
 BNA_F
 ClientSampleId :
 MW-2

Tgt Ion:165 Resp: 29328
 Ion Ratio Lower Upper
 165 100
 63 0.0 51.8 77.8#
 89 2.0 53.7 80.5#

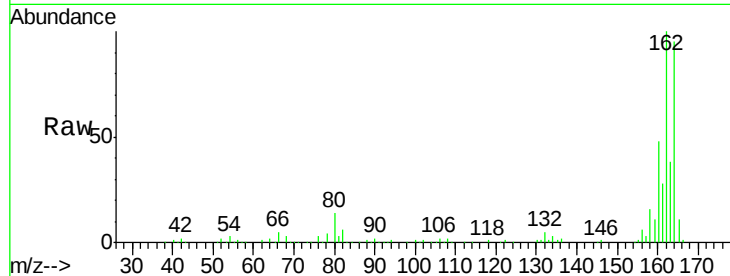




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0

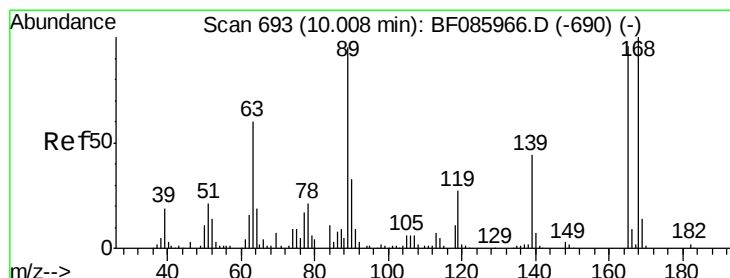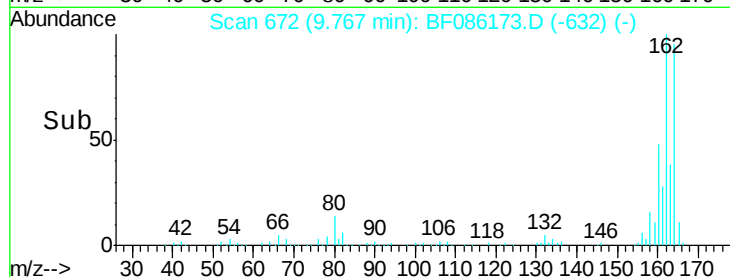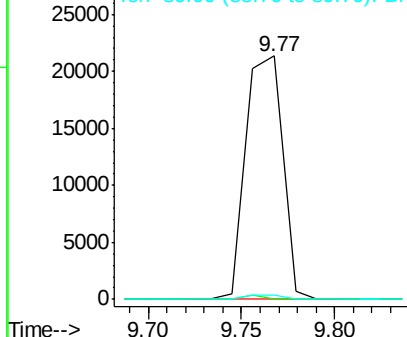


#56
 2,4-Dinitrotoluene
 Concen: 6.16 ng
 RT: 9.77 min Scan# 672
 Delta R.T. -0.24 min
 Lab File: BF086173.D
 Acq: 8 Apr 2016 17:34

Tgt Ion:165 Resp: 29328
 Ion Ratio Lower Upper
 165 100
 63 0.0 24.9 37.3#
 89 2.0 41.0 61.6#
 182 0.0 2.1 3.1#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E


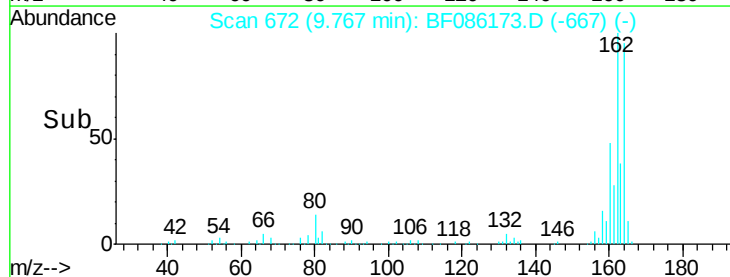
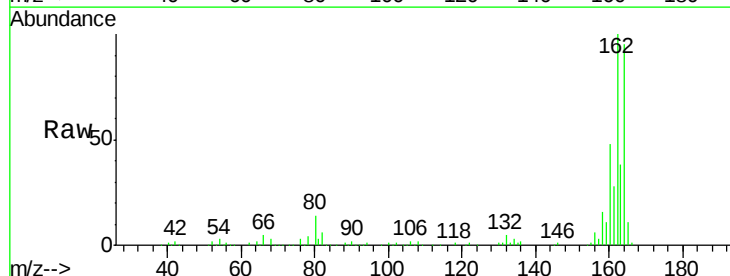
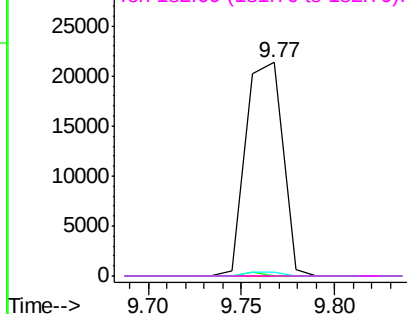


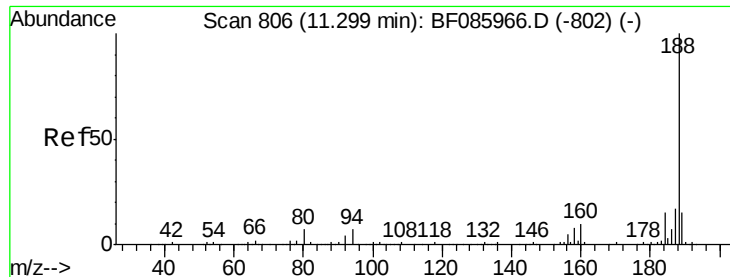

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.24 min Scan# 801
Delta R.T. -0.06 min
Lab File: BF086173.D
Acq: 8 Apr 2016 17:34




Instrument :
BNA_F
ClientSampleId :
MW-2


Tgt Ion:188 Resp: 458152
Ion Ratio Lower Upper
188 100
94 11.6 5.4 8.0#
80 12.3 5.5 8.3#

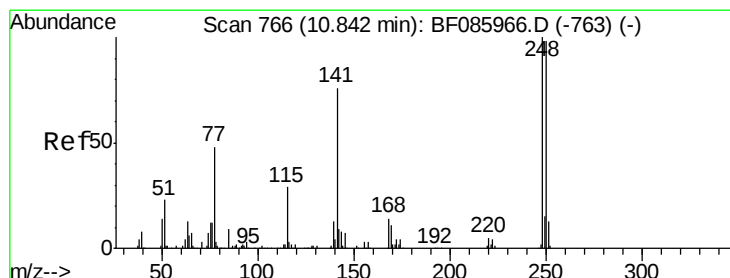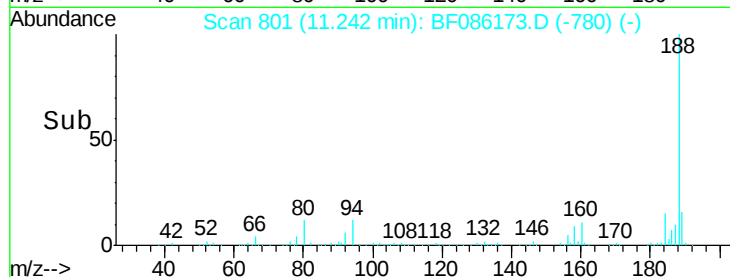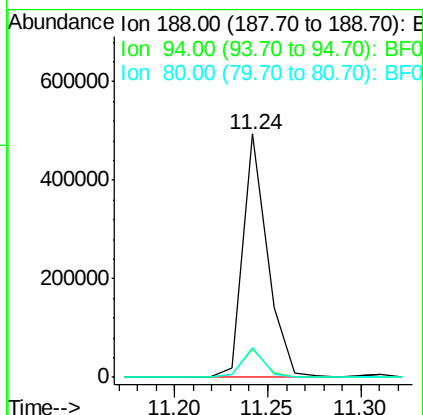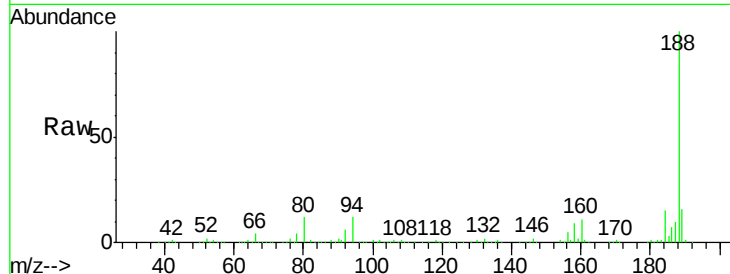

#66
4-Bromophenyl-phenylether
Concen: 4.63 ng
RT: 10.56 min Scan# 741
Delta R.T. -0.29 min
Lab File: BF086173.D
Acq: 8 Apr 2016 17:34

Tgt Ion:248 Resp: 21671
Ion Ratio Lower Upper
248 100
250 196.0 77.4 116.0#
141 390.3 63.6 95.4#

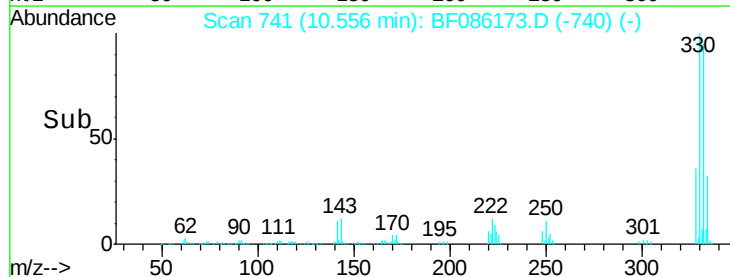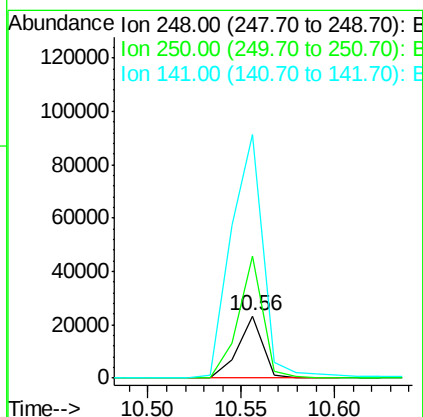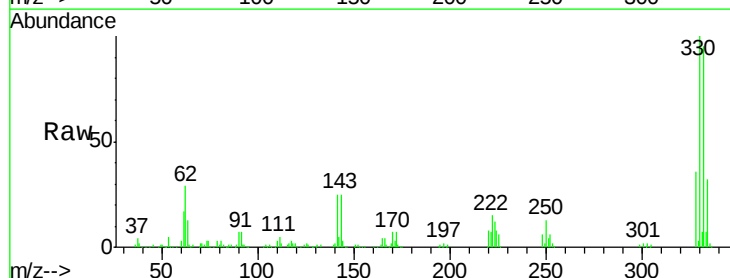

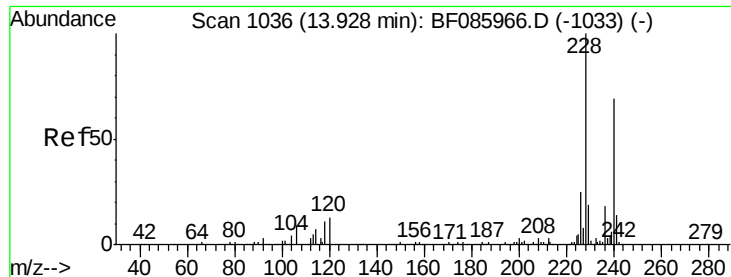

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.88 min Scan# 1032

Delta R.T. -0.05 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34

Instrument :

BNA_F

ClientSampleId :

MW-2





Tgt Ion:240 Resp: 348421

Ion Ratio Lower Upper

240 100

120 10.3 13.8 20.8#

236 27.1 20.6 30.8

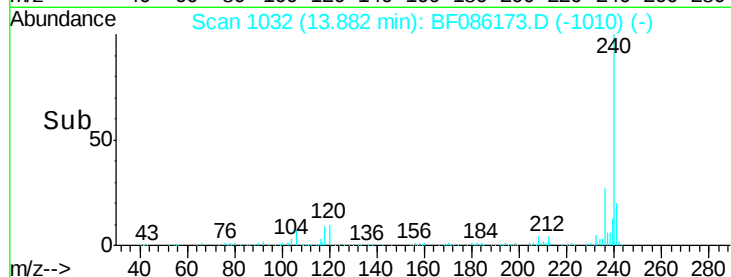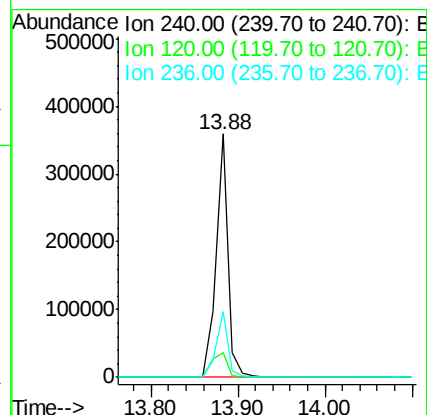

#78

Terphenyl-d14

Concen: 80.99 ng

RT: 12.83 min Scan# 940

Delta R.T. -0.05 min

Lab File: BF086173.D

Acq: 8 Apr 2016 17:34




Tgt Ion:244 Resp: 1200481




Ion Ratio Lower Upper

244 100

212 7.3 6.1 9.1

122 11.2 10.2 15.4

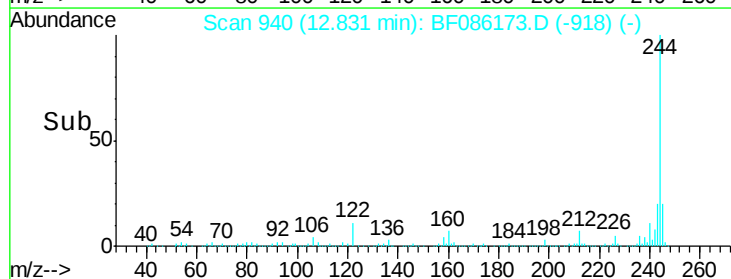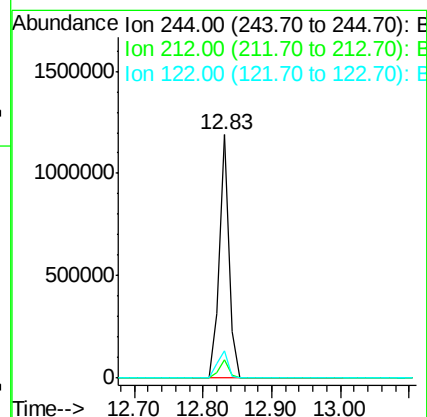

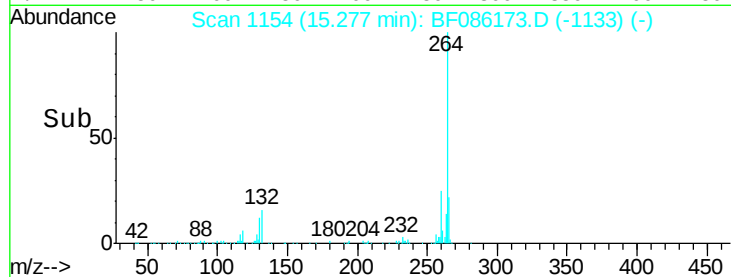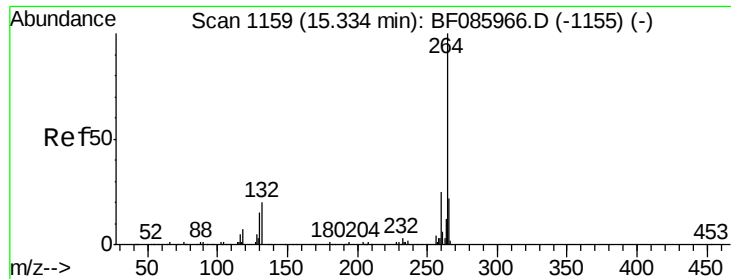

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.28 min Scan# 1154
Delta R.T. -0.06 min
Lab File: BF086173.D
Acq: 8 Apr 2016 17:34

Instrument :
BNA_F
ClientSampleId :
MW-2

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.4	29.2
265	21.5	17.2	25.8

