
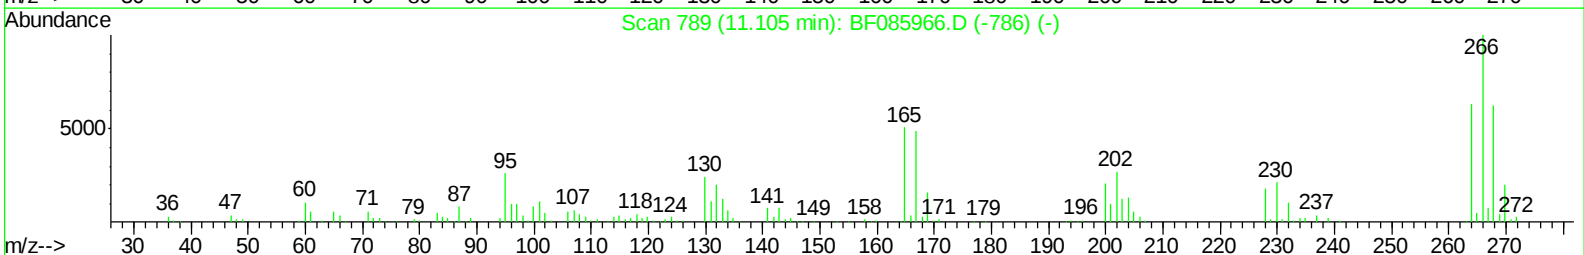
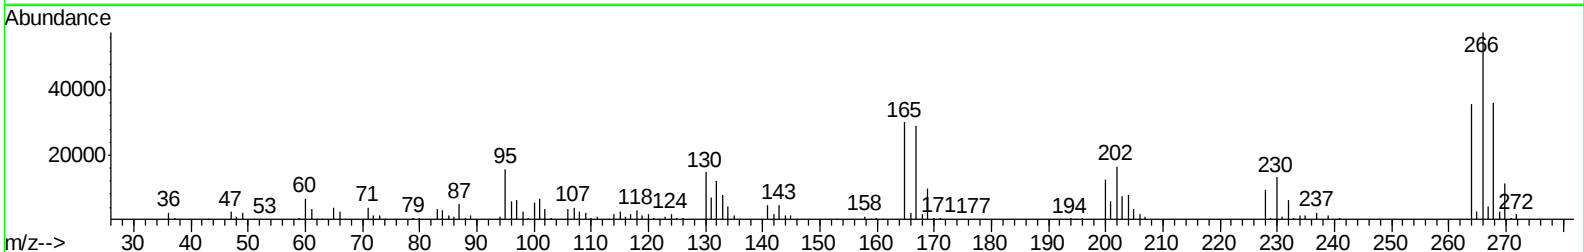


```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF040816\  
Data File : BF086162.D  
Acq On    : 8 Apr 2016 11:35  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Apr 11 07:38:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

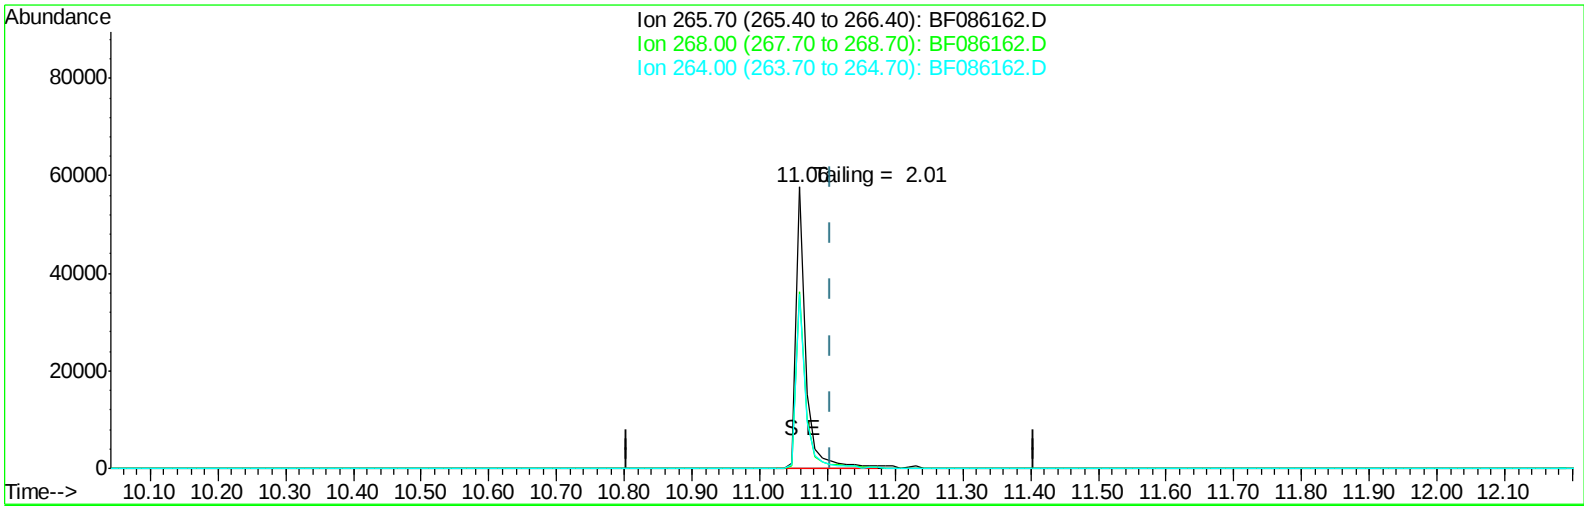

TIC: BF086162.D

(69) Pentachlorophenol (C)




11.059min (-0.046) 37687.50ng

response 59300

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.88
264.00	63.30	61.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040816\
Data File : BF086162.D
Acq On : 8 Apr 2016 11:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 07:38:29 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

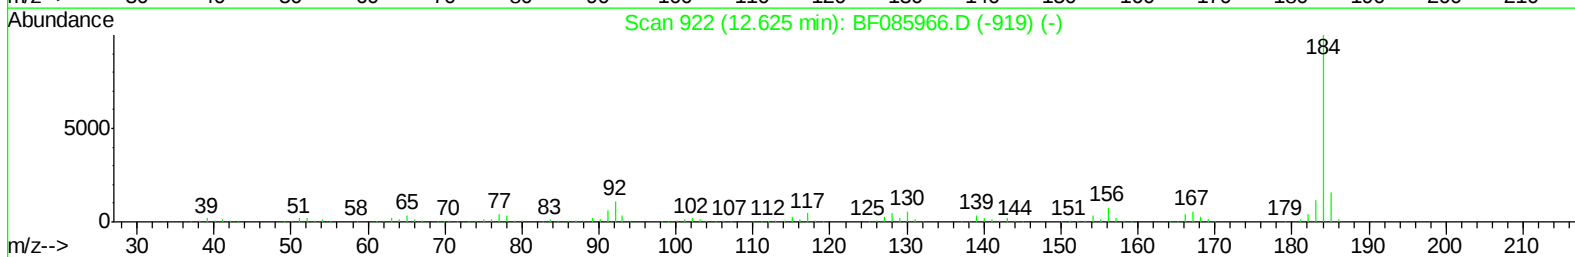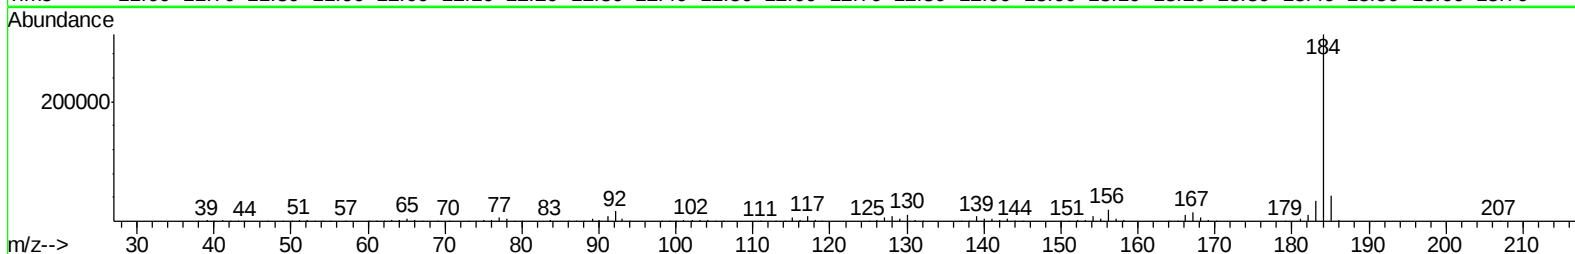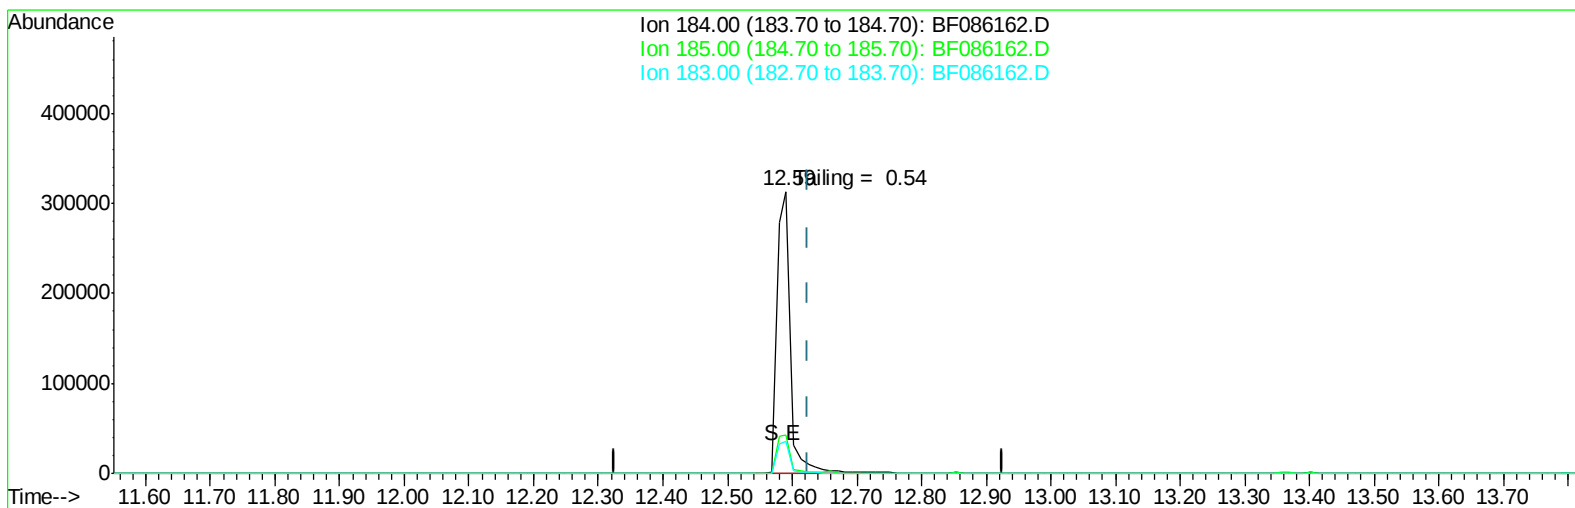

TIC: BF086162.D

(76) Benzidine

12.591min (-0.034) 0.00ng

response 467252

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.56
183.00	11.80	11.33
0.00	0.00	0.00