

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
 Data File : BF086173.D
 Acq On : 8 Apr 2016 17:34
 Operator : UM/SJ
 Sample : H2343-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	244	246	261	rBV	39459	70290	1.72%	0.271%
2	5.321	281	283	301	rBV	1492697	1633697	39.96%	6.299%
3	6.373	373	375	383	rBV	1030462	1117398	27.33%	4.308%
4	6.499	383	386	388	rBV	2547262	2760528	67.53%	10.643%
5	6.727	404	406	412	rBV	758415	724630	17.73%	2.794%
6	6.876	417	419	422	rBV	1765000	2480990	60.69%	9.566%
7	7.299	453	456	458	rBV	2059693	2098253	51.33%	8.090%
8	8.007	516	518	521	rBV	827119	962581	23.55%	3.711%
9	9.093	610	613	615	rBV	3624253	4088153	100.00%	15.762%
10	9.493	646	648	650	rBV	61381	69923	1.71%	0.270%
11	9.767	669	672	674	rBV	841763	1114097	27.25%	4.296%
12	10.190	708	709	711	rVB	38925	52283	1.28%	0.202%
13	10.556	738	741	743	rBV	2268232	2359058	57.70%	9.096%
14	10.670	749	751	757	rVB	60739	83889	2.05%	0.323%
15	11.242	799	801	804	rBV	1259461	1150362	28.14%	4.435%
16	12.831	937	940	943	rBV	3461050	3547087	86.77%	13.676%
17	13.882	1029	1032	1034	rBV	938954	950896	23.26%	3.666%
18	15.277	1151	1154	1163	rBV	492771	672215	16.44%	2.592%


Sum of corrected areas: 25936330

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
Data File : BF086173.D
Acq On : 8 Apr 2016 17:34
Operator : UM/SJ
Sample : H2343-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

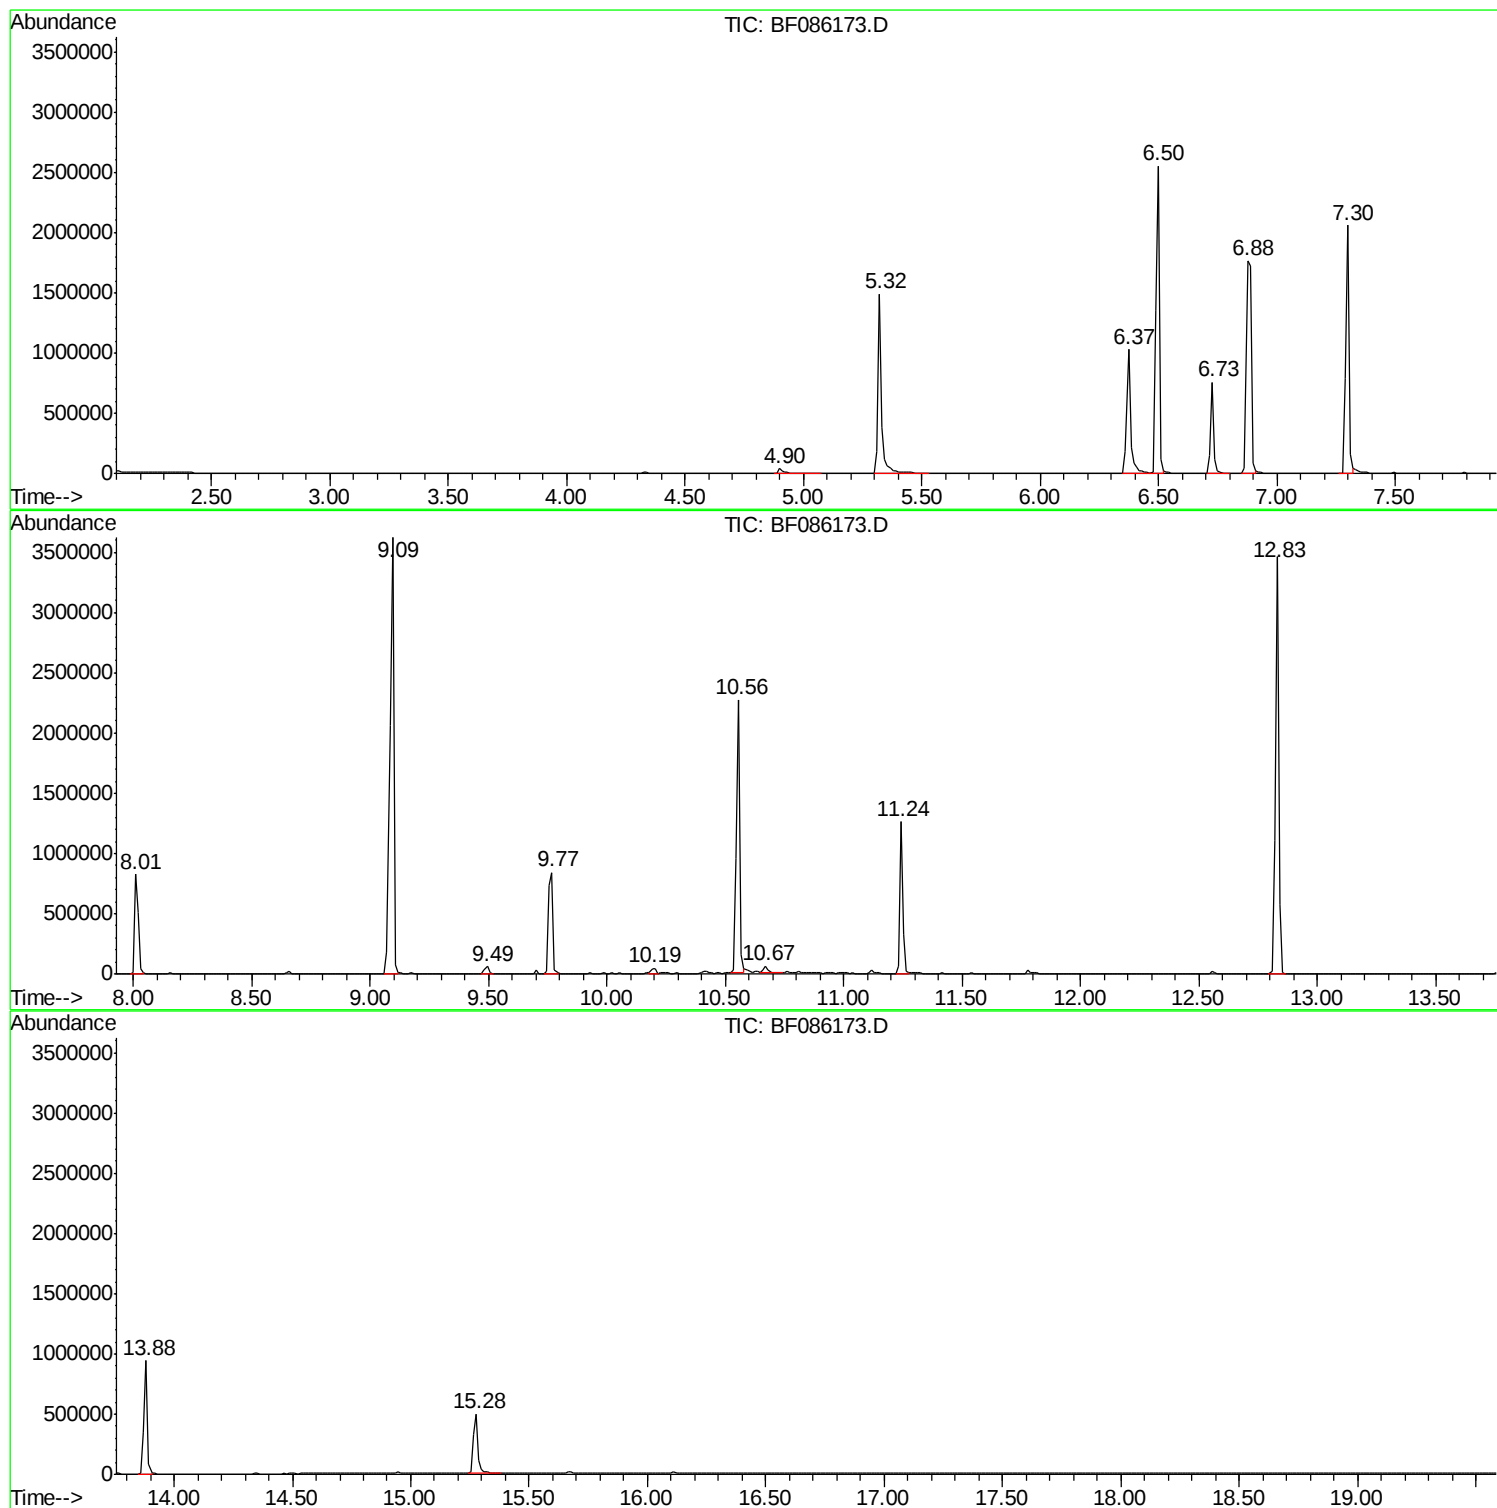

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
Data File : BF086173.D
Acq On : 8 Apr 2016 17:34
Operator : UM/SJ
Sample : H2343-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
Data File : BF086173.D
Acq On : 8 Apr 2016 17:34
Operator : UM/SJ
Sample : H2343-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc