

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
 Data File : BF086174.D
 Acq On : 8 Apr 2016 18:03
 Operator : UM/SJ
 Sample : H2343-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	244	246	255	rBV	39132	69531	1.72%	0.273%
2	5.321	281	283	300	rBV	1404622	1521030	37.67%	5.981%
3	6.373	373	375	383	rBV	896390	1016862	25.19%	3.998%
4	6.499	383	386	388	rBV	2375227	2665076	66.01%	10.479%
5	6.727	404	406	412	rBV	745952	720294	17.84%	2.832%
6	6.876	417	419	422	rBV	1892700	2424642	60.06%	9.534%
7	7.299	453	456	458	rBV	2005367	2115156	52.39%	8.317%
8	8.007	516	518	521	rBV	897793	968588	23.99%	3.808%
9	9.093	610	613	615	rBV	3401557	4037285	100.00%	15.874%
10	9.493	645	648	650	rBV	61117	76756	1.90%	0.302%
11	9.756	669	671	674	rBV	794109	1103098	27.32%	4.337%
12	10.202	708	710	711	rVB	37768	49186	1.22%	0.193%
13	10.556	738	741	743	rBV	2250950	2297120	56.90%	9.032%
14	10.670	749	751	758	rVB	60765	81917	2.03%	0.322%
15	11.242	799	801	804	rBV	1214741	1140300	28.24%	4.484%
16	11.779	846	848	850	rBV	45184	51534	1.28%	0.203%
17	12.831	937	940	943	rBV	3464740	3432701	85.02%	13.497%
18	13.882	1029	1032	1034	rBV	920520	975058	24.15%	3.834%
19	15.277	1151	1154	1159	rBV	480311	686619	17.01%	2.700%


Sum of corrected areas: 25432753

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
Data File : BF086174.D
Acq On : 8 Apr 2016 18:03
Operator : UM/SJ
Sample : H2343-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

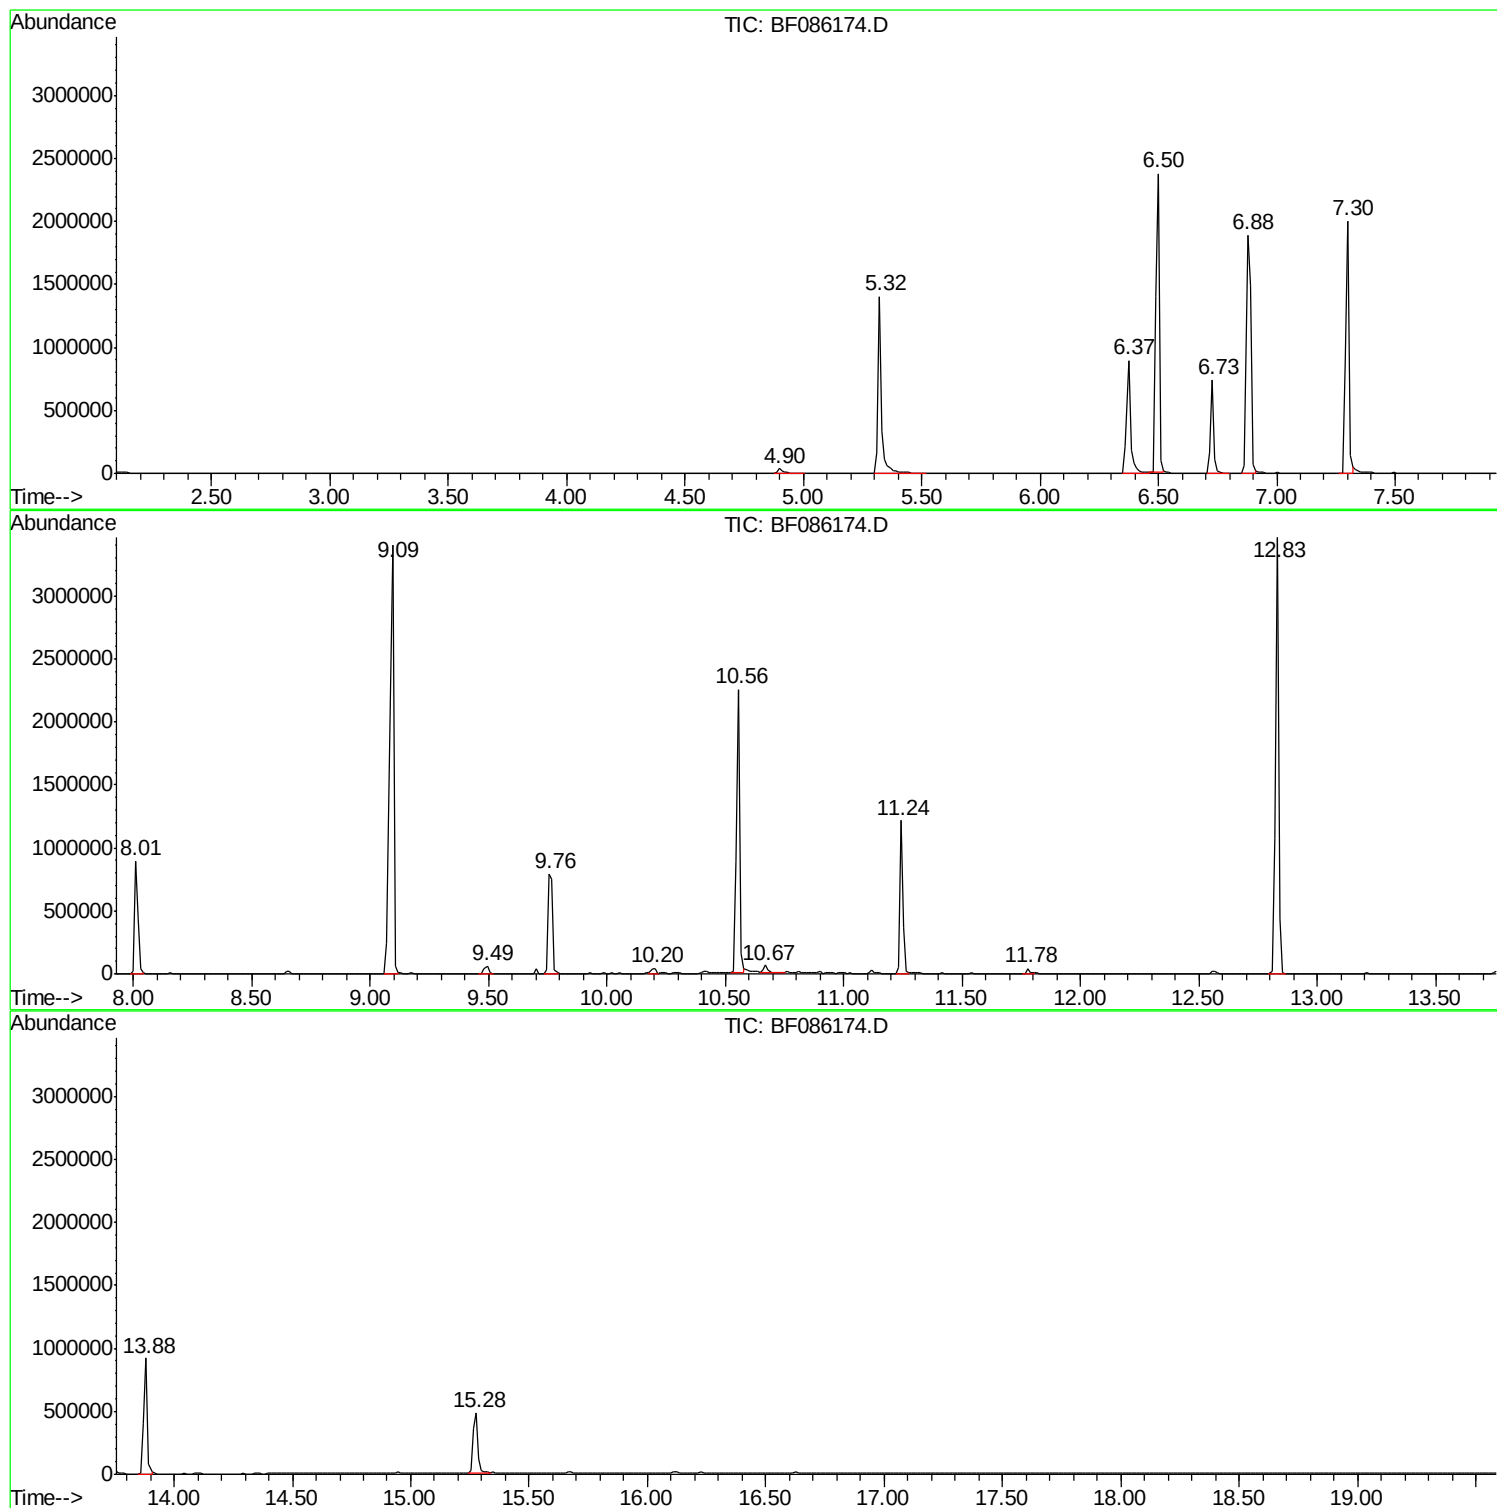

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
Data File : BF086174.D
Acq On : 8 Apr 2016 18:03
Operator : UM/SJ
Sample : H2343-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	74.00 ng	2665080	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

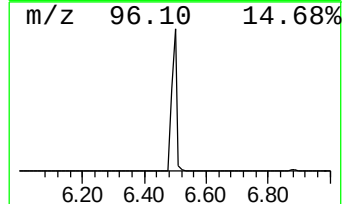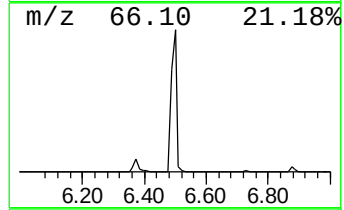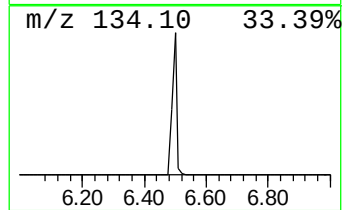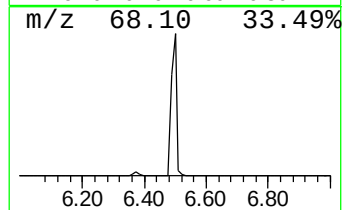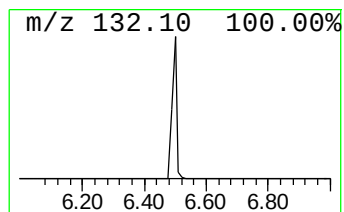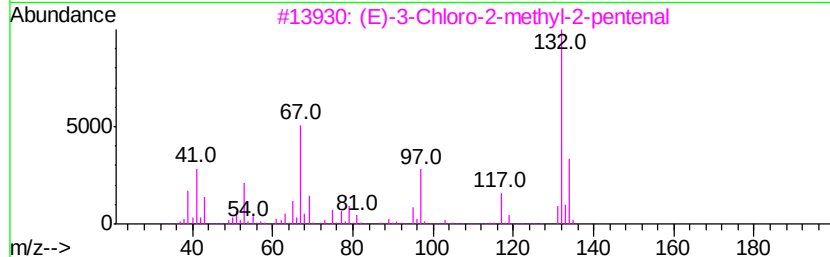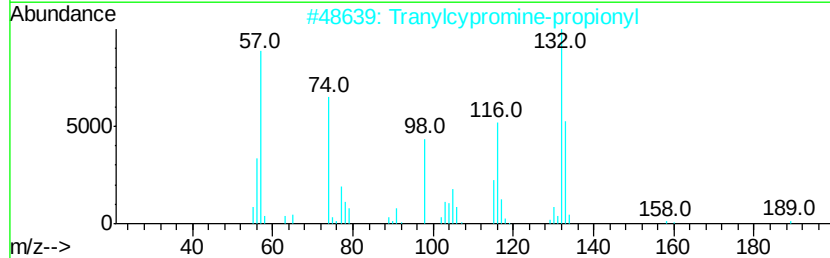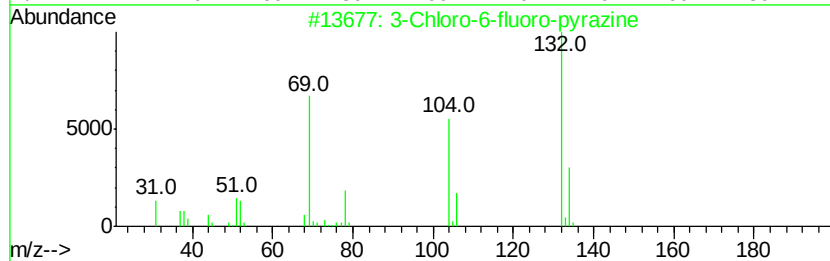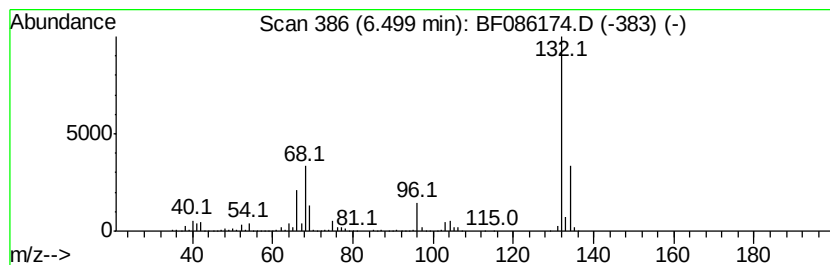

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040816\
Data File : BF086174.D
Acq On : 8 Apr 2016 18:03
Operator : UM/SJ
Sample : H2343-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	74.0	ng	2665080	1	6.73	720294	20.0