


Data Path : Z:\HPCHEM1\BNA F\Data\BF040816\
 Data File : BF086162.D
 Acq On : 8 Apr 2016 11:35
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 01 23:17:06 2016

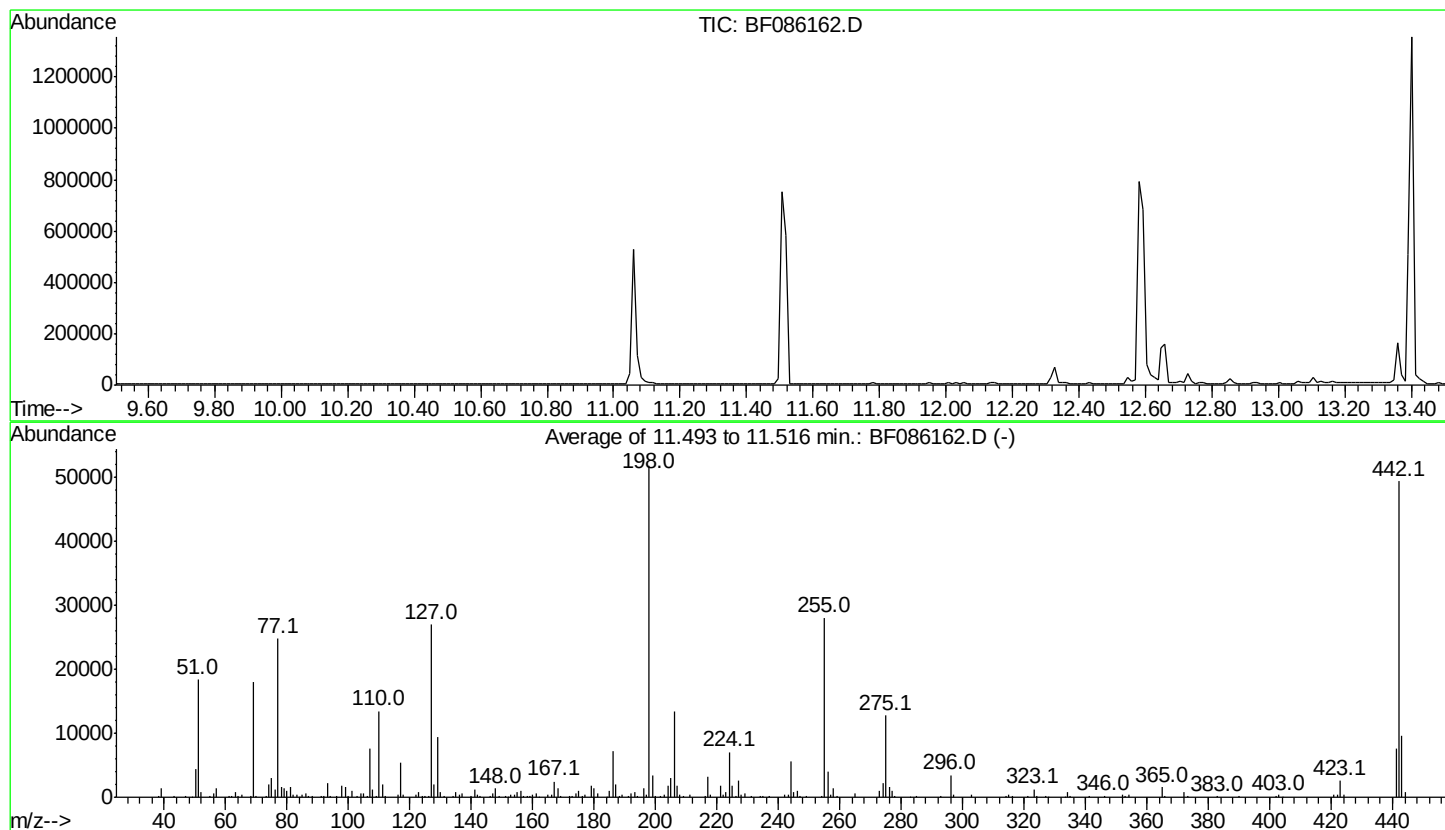

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	18405	PASS
68	69	0.00	2	1.4	247	PASS
69	198	0.00	100	34.8	18045	PASS
70	69	0.00	2	0.6	110	PASS
127	198	10	80	52.1	27005	PASS
197	198	0.00	2	0.8	393	PASS
198	198	100	100	100.0	51877	PASS
199	198	5	9	6.7	3468	PASS
275	198	10	60	24.6	12757	PASS
365	198	1	100	3.1	1586	PASS
441	442	0.01	24	15.6	7693	PASS
442	198	50	100	95.3	49421	PASS
443	442	15	24	19.4	9599	PASS