


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF040816\  
 Data File : BF086183.D  
 Acq On : 8 Apr 2016 22:16  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF040216.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Apr 01 23:17:06 2016

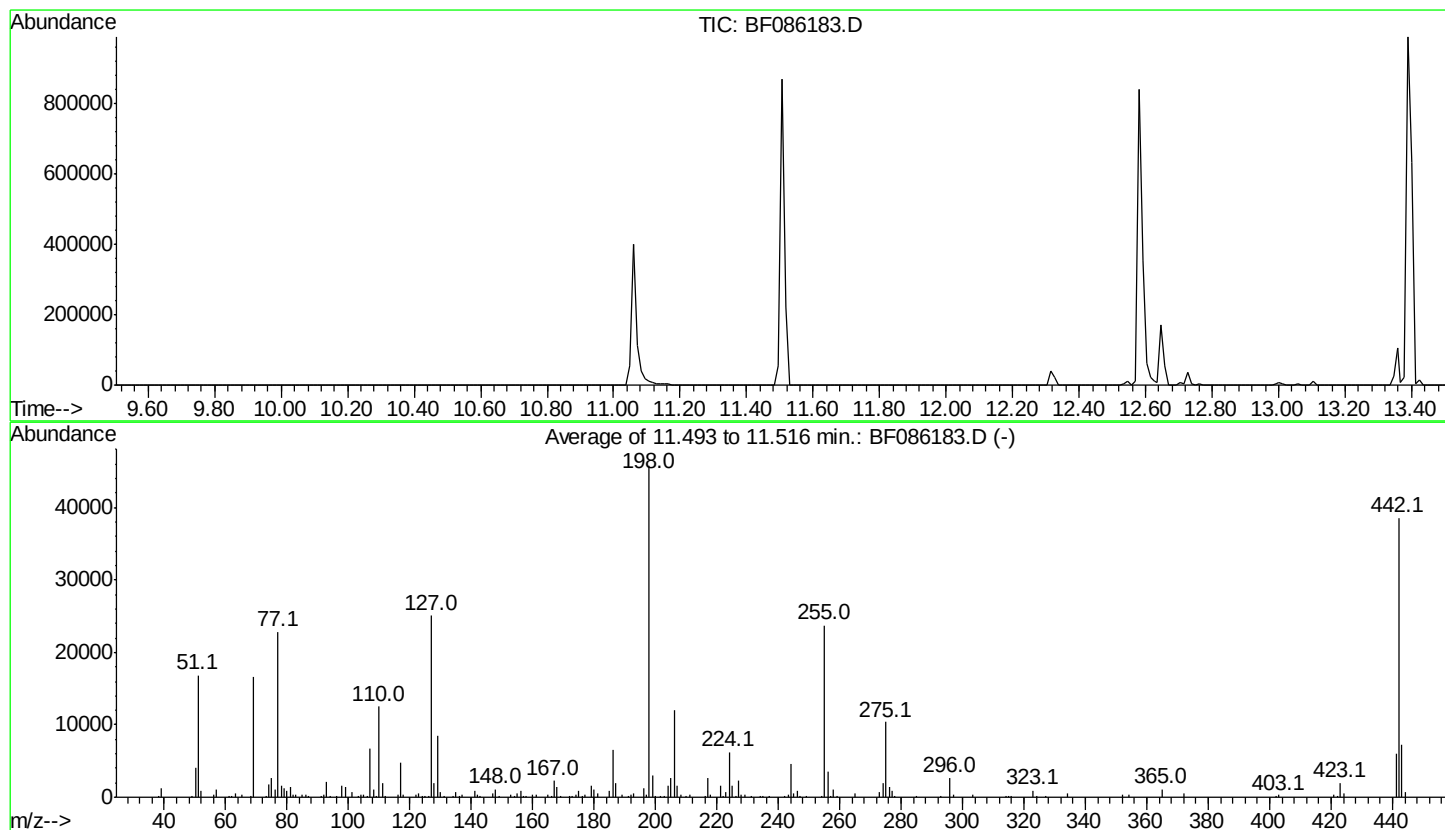

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.7      | 16808   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 233     | PASS             |
| 69          | 198          | 0.00         | 100          | 36.3      | 16600   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 54.7      | 25062   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 276     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 45792   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 3038    | PASS             |
| 275         | 198          | 10           | 60           | 22.7      | 10396   | PASS             |
| 365         | 198          | 1            | 100          | 2.5       | 1145    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.5      | 5962    | PASS             |
| 442         | 198          | 50           | 100          | 84.2      | 38557   | PASS             |
| 443         | 442          | 15           | 24           | 18.7      | 7204    | PASS             |