
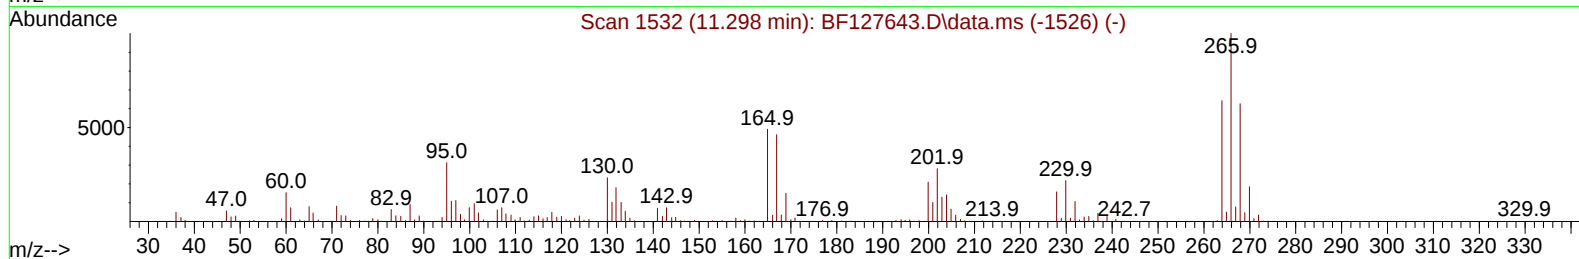
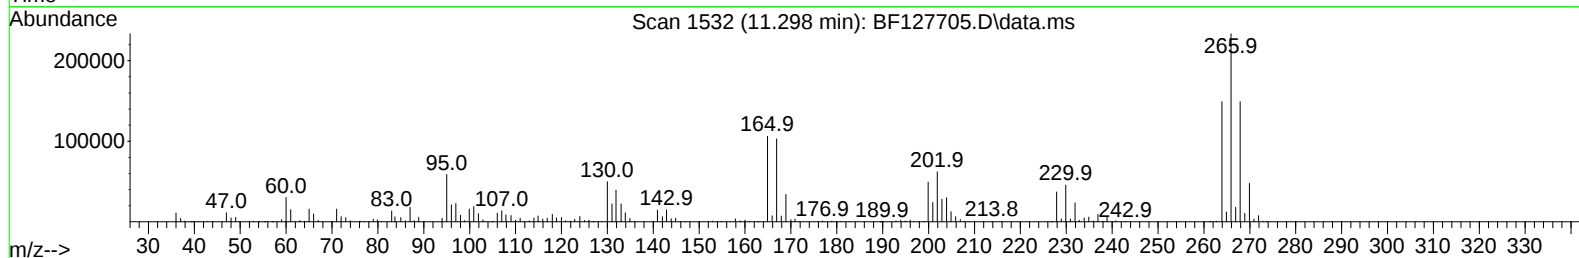


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040822\  
Data File : BF127705.D  
Acq On : 08 Apr 2022 10:05  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 03:27:13 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 06 13:55:27 2022  
Response via : Initial Calibration

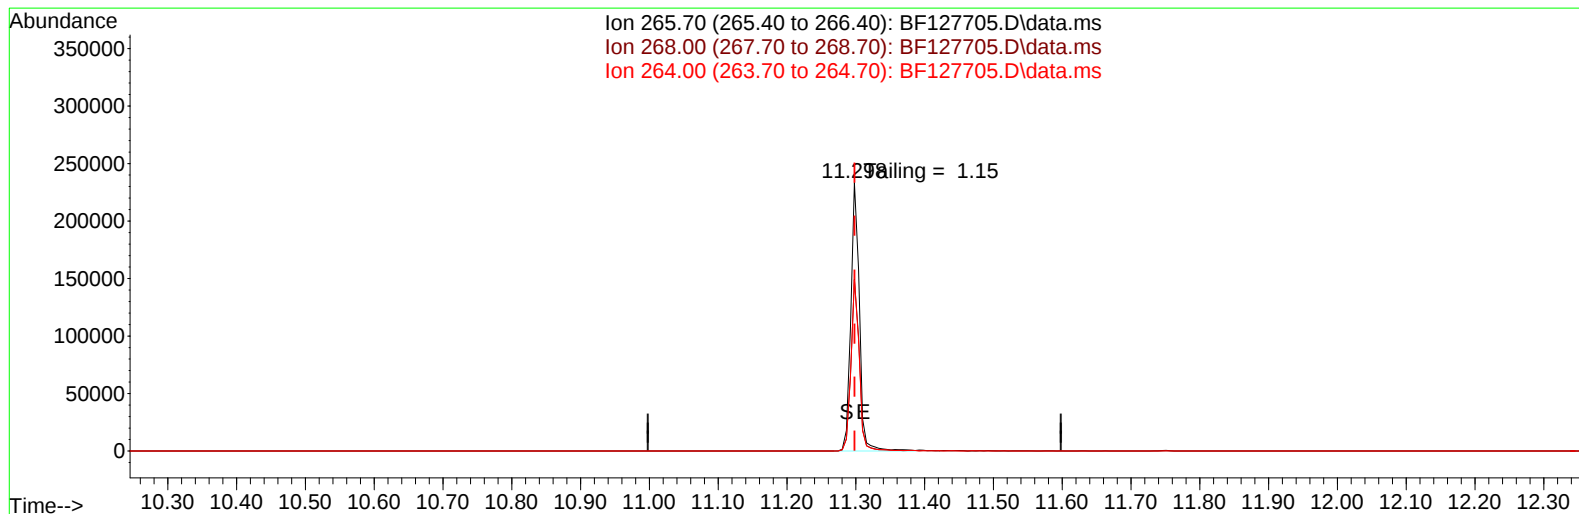




TIC: BF127705.D\data.ms

**(70) Pentachlorophenol (C)****11.298min (-0.000) 476557.09 ng****response 200133**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 63.86  |
| 264.00 | 60.60  | 63.83  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040822\  
Data File : BF127705.D  
Acq On : 08 Apr 2022 10:05  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 03:27:13 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 06 13:55:27 2022  
Response via : Initial Calibration

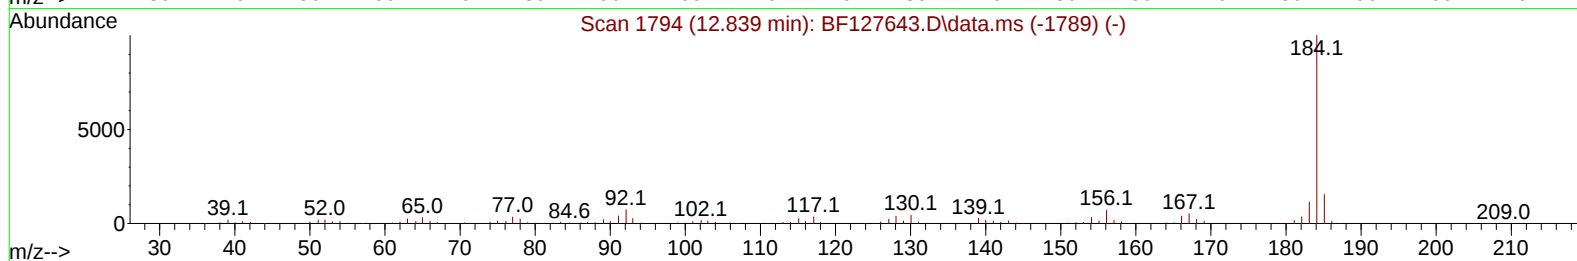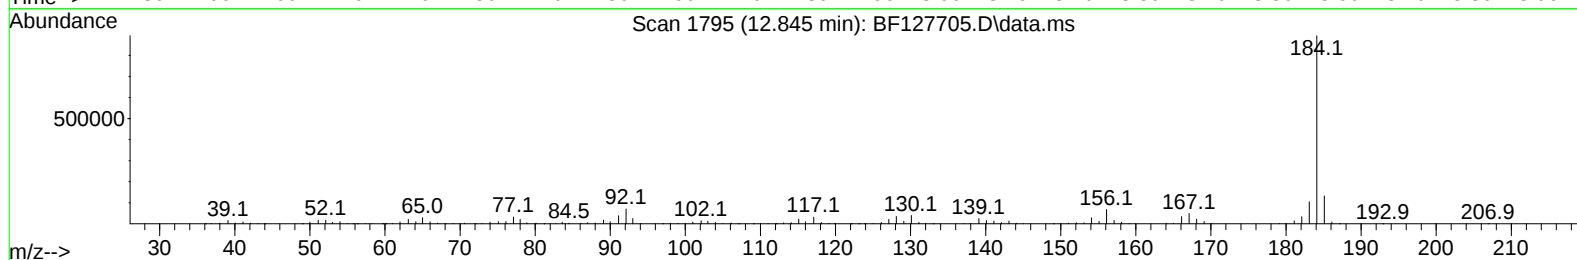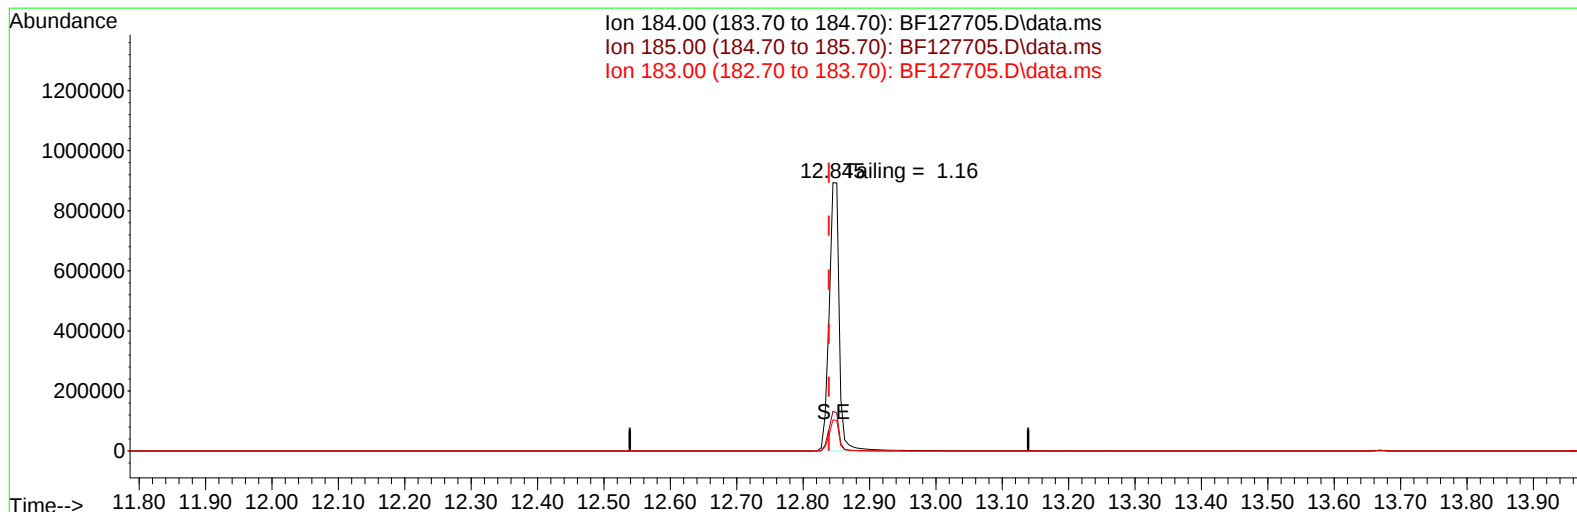

TIC: BF127705.D\data.ms

**(77) Benzidine****12.845min (+ 0.006) 157862.18 ng****response 947672**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.84  |
| 183.00 | 11.70  | 11.66  |
| 0.00   | 0.00   | 0.00   |