
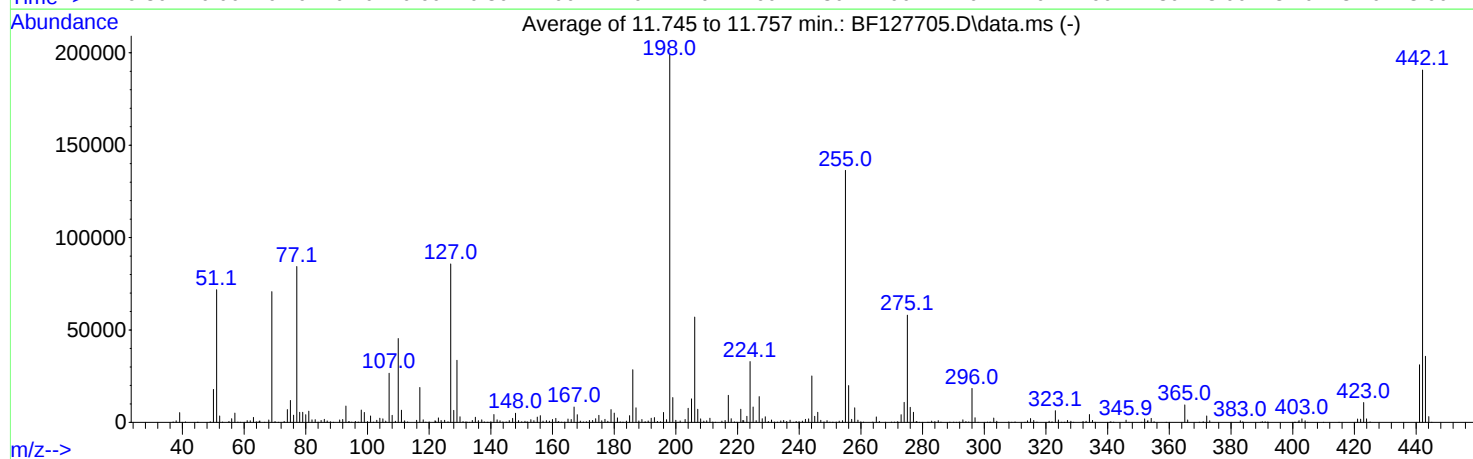


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040822\
 Data File : BF127705.D
 Acq On : 08 Apr 2022 10:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 06 13:55:27 2022

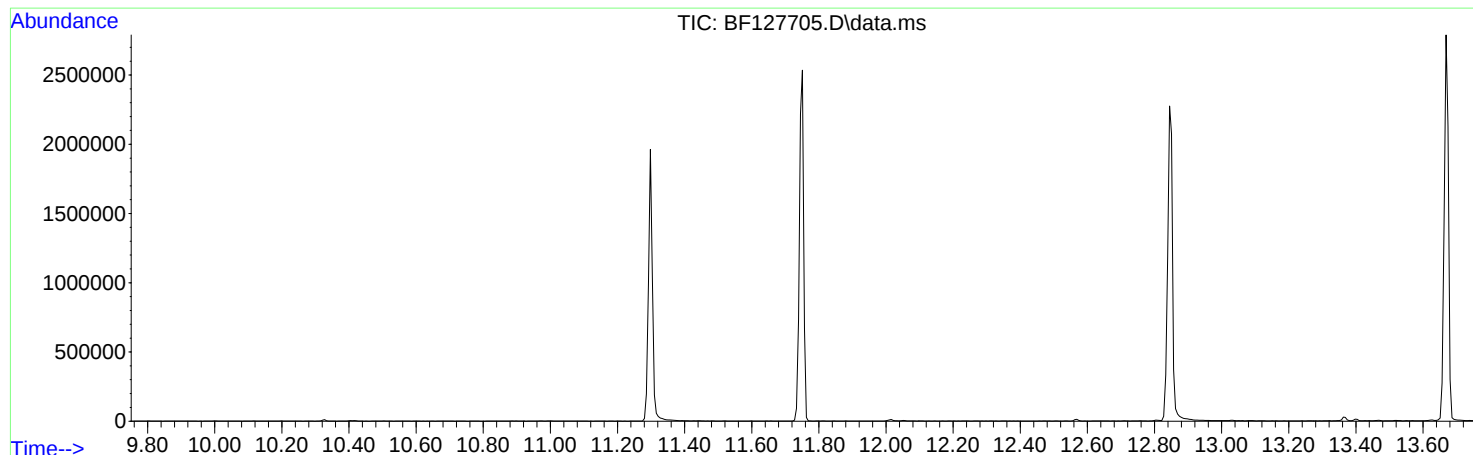




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	71764	PASS
68	69	0.00	2	1.8	1271	PASS
69	198	0.00	100	35.5	70758	PASS
70	69	0.00	2	0.6	433	PASS
127	198	10	80	43.1	85715	PASS
197	198	0.00	2	0.7	1457	PASS
198	198	100	100	100.0	199059	PASS
199	198	5	9	6.7	13428	PASS
275	198	10	60	29.1	58000	PASS
365	198	1	100	4.7	9447	PASS
441	198	0.01	100	15.7	31213	PASS
442	442	50	100	100.0	190677	PASS
443	442	15	24	18.8	35803	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040822\
Data File : BF127705.D
Acq On : 08 Apr 2022 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 11 03:27:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:55:27 2022
Response via : Initial Calibration

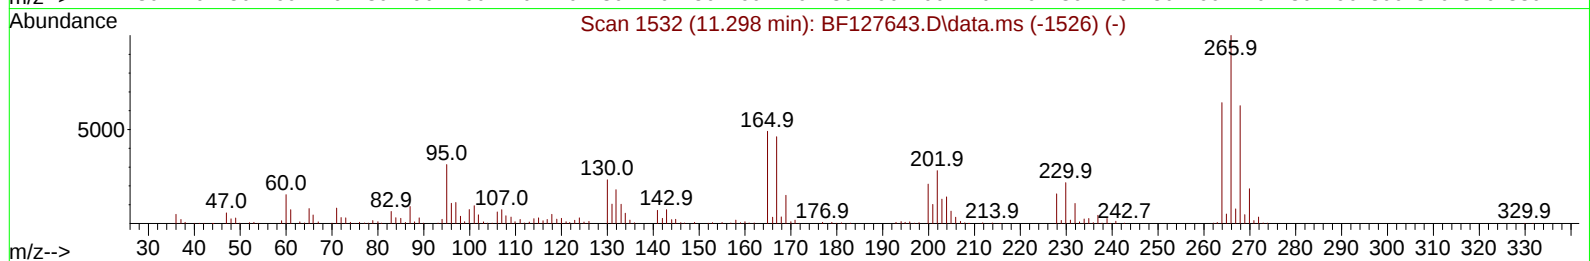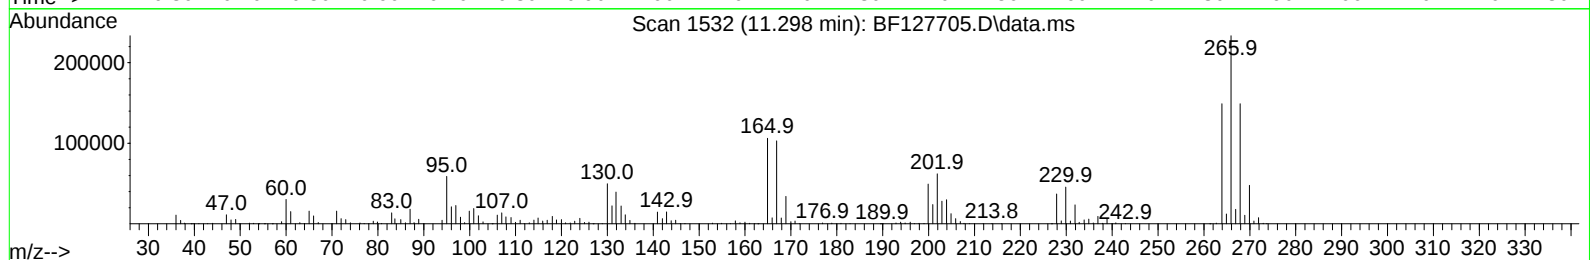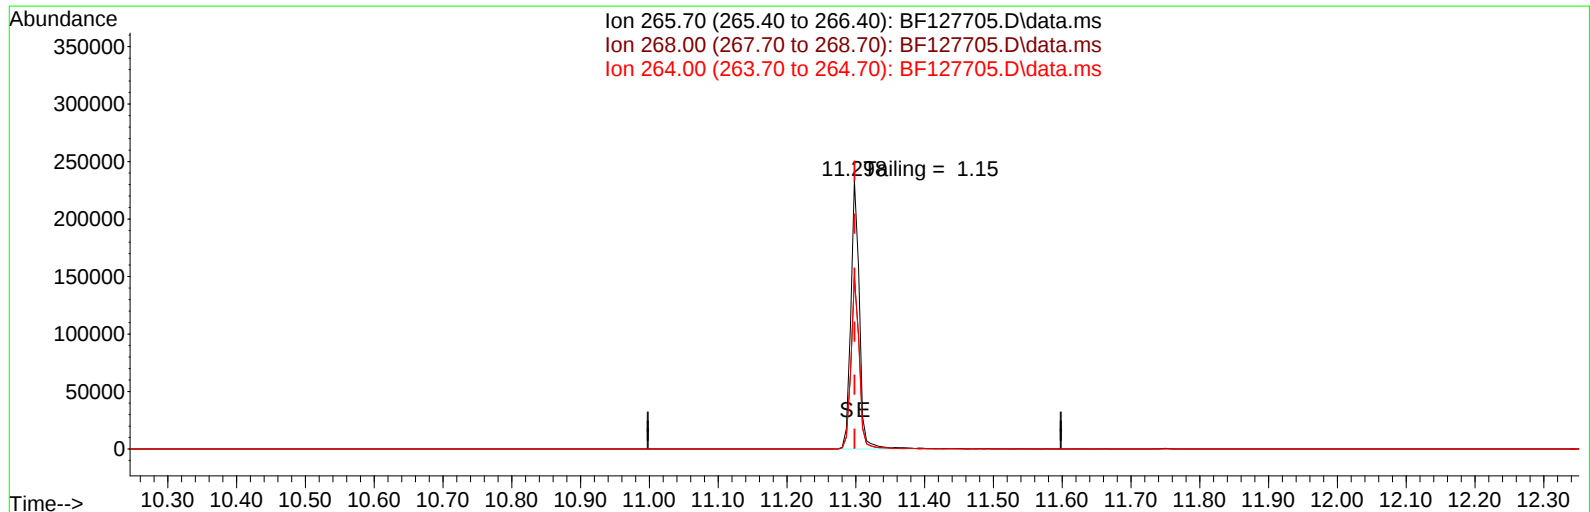

TIC: BF127705.D\data.ms

(70) Pentachlorophenol (C)

11.298min (-0.000) 476557.09 ng




response 200133

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.86
264.00	60.60	63.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040822\
Data File : BF127705.D
Acq On : 08 Apr 2022 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 11 03:27:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:55:27 2022
Response via : Initial Calibration

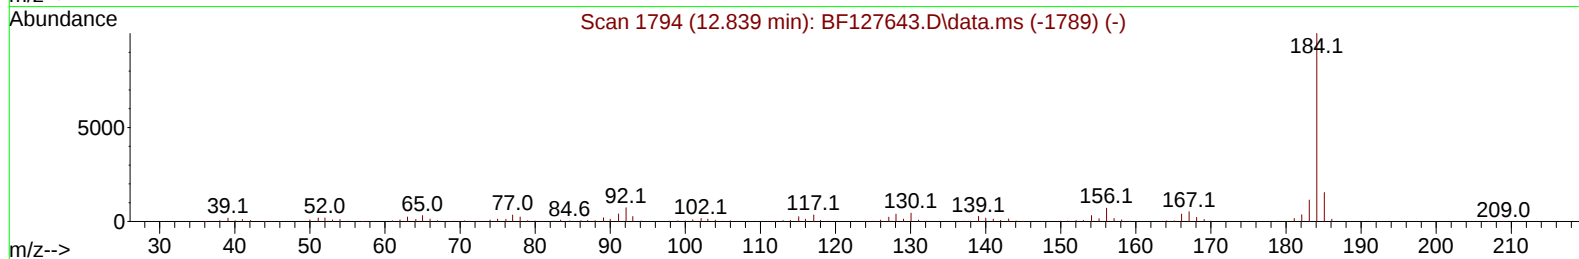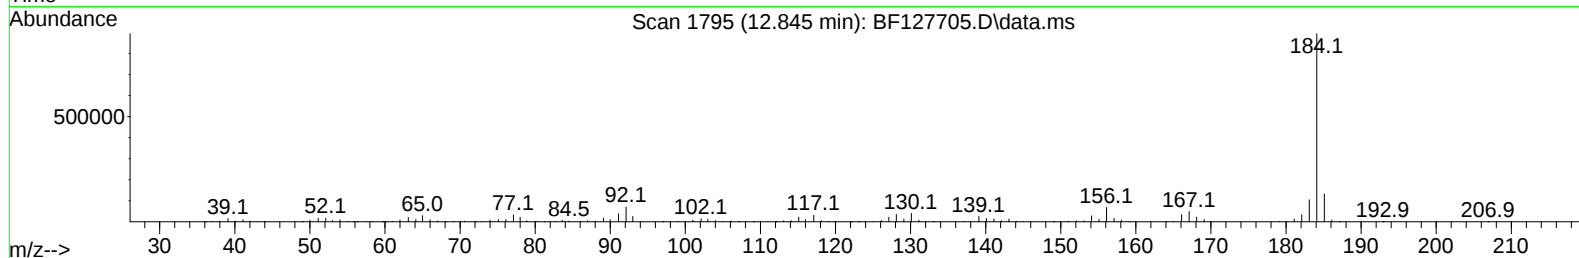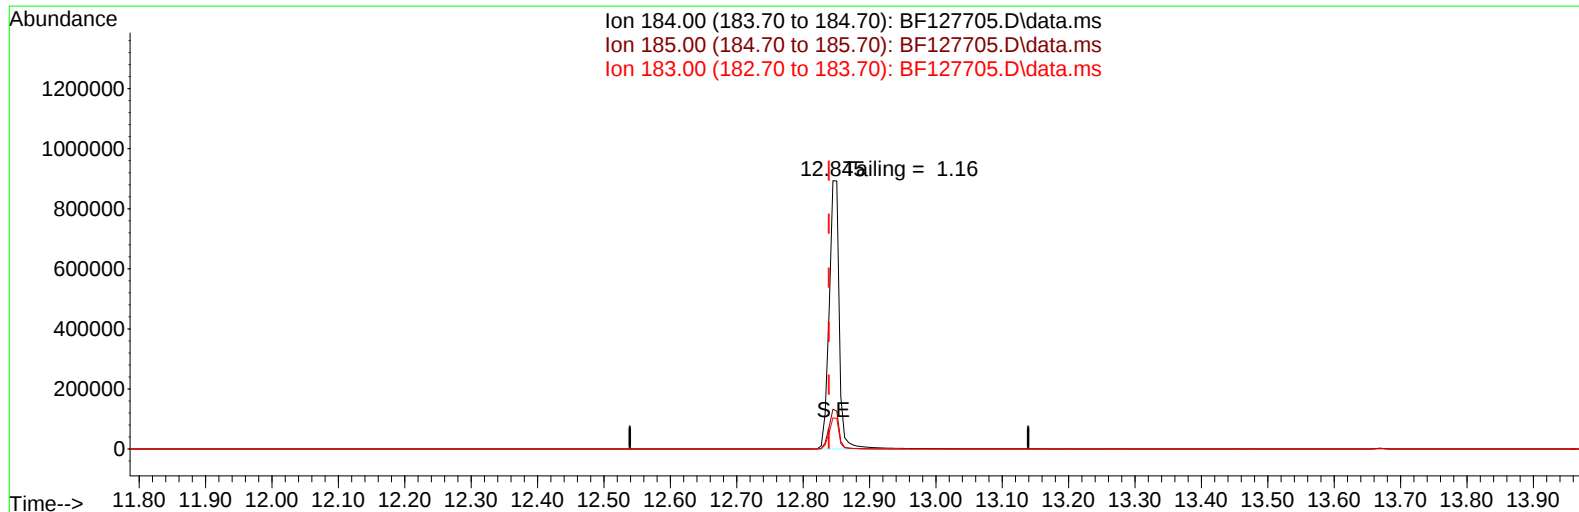

TIC: BF127705.D\data.ms

(77) Benzidine

12.845min (+ 0.006) 157862.18 ng

response 947672

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.84
183.00	11.70	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2022	BNA_F	<u>BF127705.D</u>
Compound Name	Response	Retention Time
DDT	464942	13.668
DDD	6986	13.368
DDE	648	13.027
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7634	472576	1.62

Instrument :
BNA_F
ClientSampleId :
DFTPP