
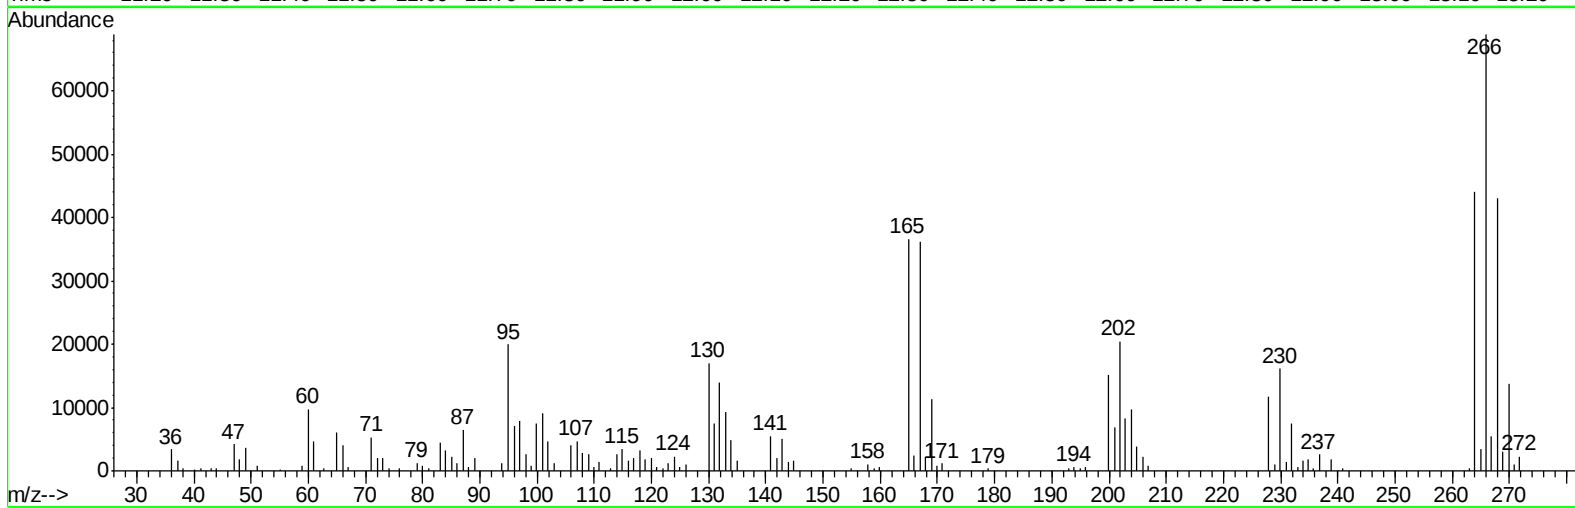


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040915\
Data File : BF078357.D
Acq On : 9 Apr 2015 11:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 07:45:00 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 10 01:53:29 2015
Response via : Initial Calibration

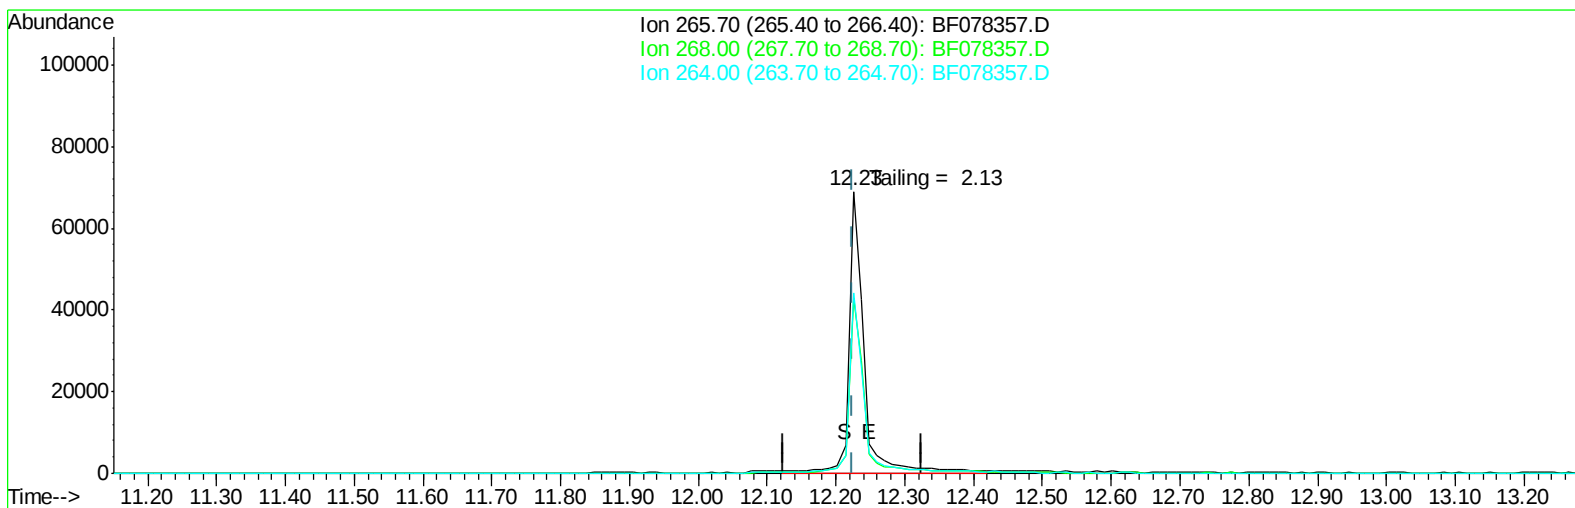

TIC: BF078357.D

(69) Pentachlorophenol (C)



12.225min (-0.000) 0.00ng

response 92582

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	62.34
264.00	62.50	64.03
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040915\
Data File : BF078357.D
Acq On : 9 Apr 2015 11:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 07:45:00 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 10 01:53:29 2015
Response via : Initial Calibration

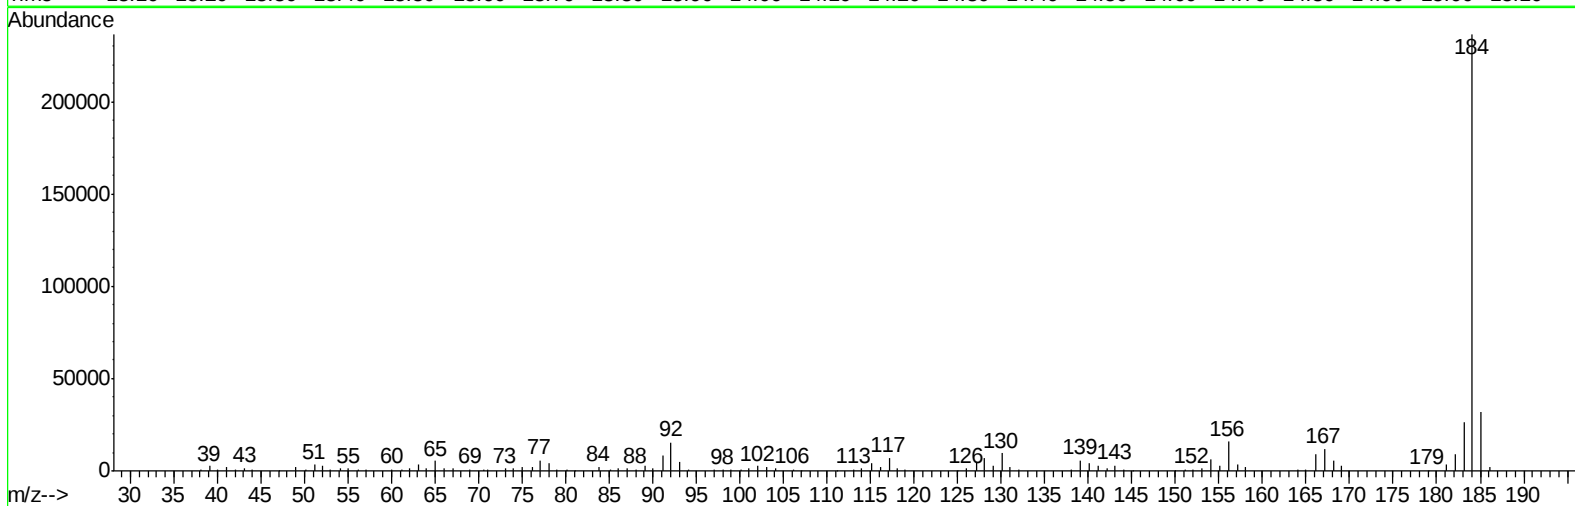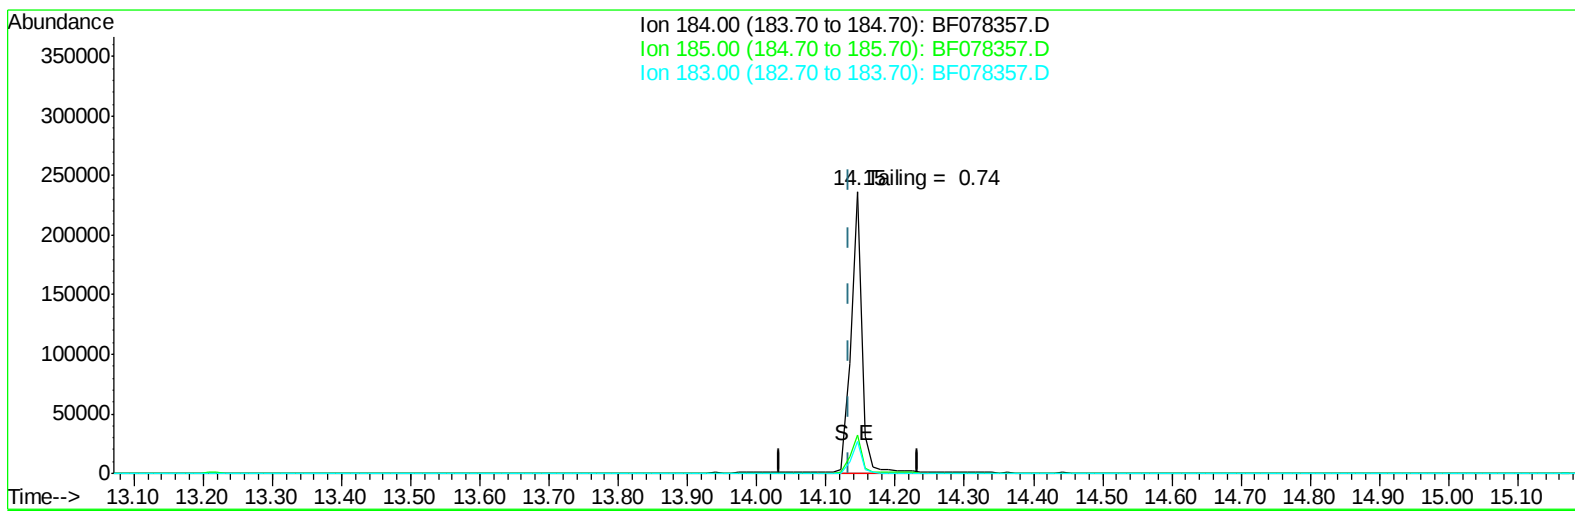

TIC: BF078357.D

(76) Benzidine

14.145min (+0.011) 0.00ng

response 253693

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.63
183.00	11.90	11.24
0.00	0.00	0.00