


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040915\
 Data File : BF078375.D
 Acq On : 10 Apr 2015 00:40
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 09 11:29:31 2015

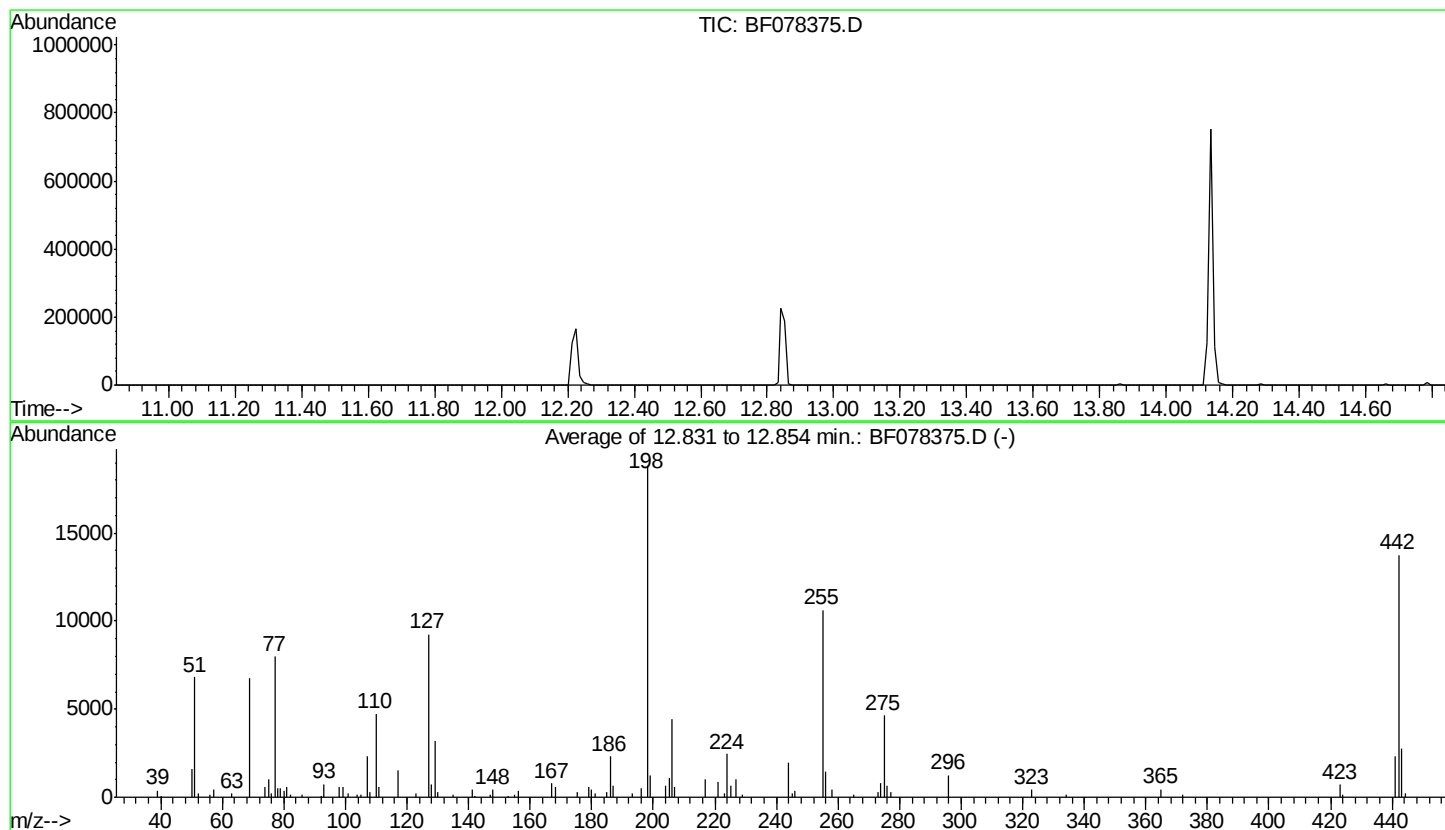

AutoFind: Scans 1045, 1046, 1047; Background Corrected with Scan 1042

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	6805	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.9	6760	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	9239	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18833	PASS
199	198	5	9	6.4	1204	PASS
275	198	10	60	24.6	4627	PASS
365	198	1	100	2.5	468	PASS
441	442	0.01	24	16.9	2327	PASS
442	198	50	100	73.1	13774	PASS
443	442	15	24	20.2	2787	PASS