
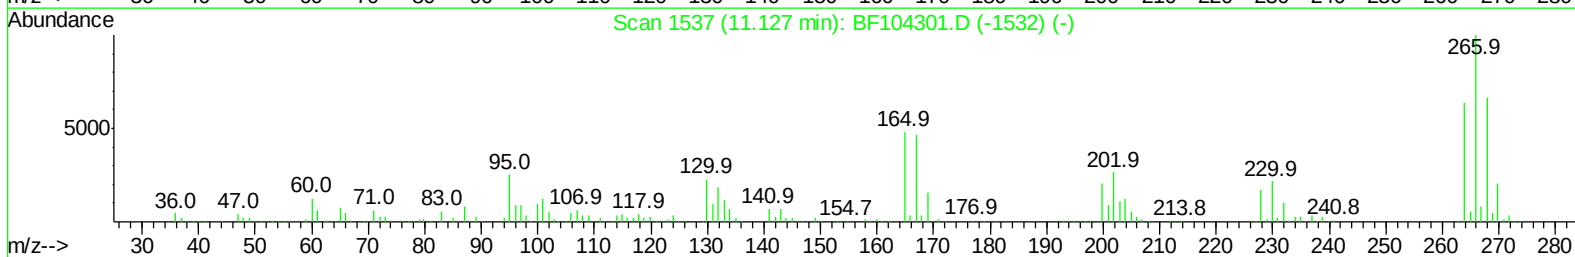
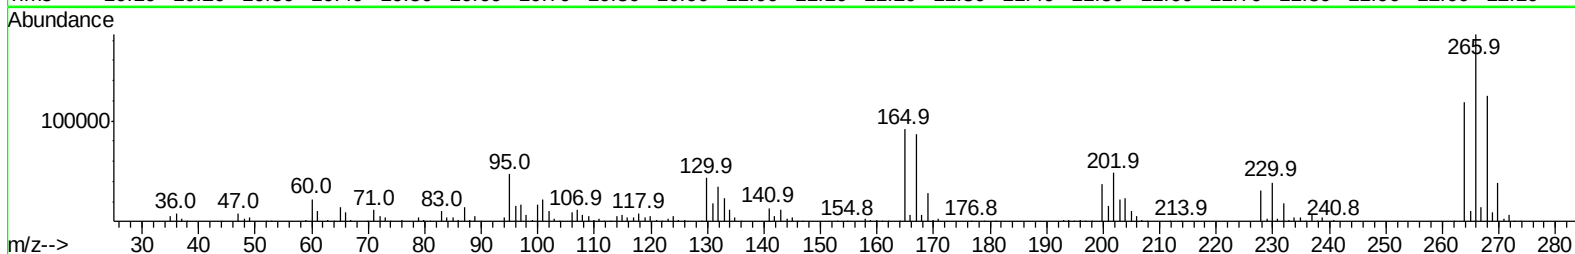


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040918\
Data File : BF104358.D
Acq On : 9 Apr 2018 8:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 04:18:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 06 16:44:53 2018
Response via : Initial Calibration

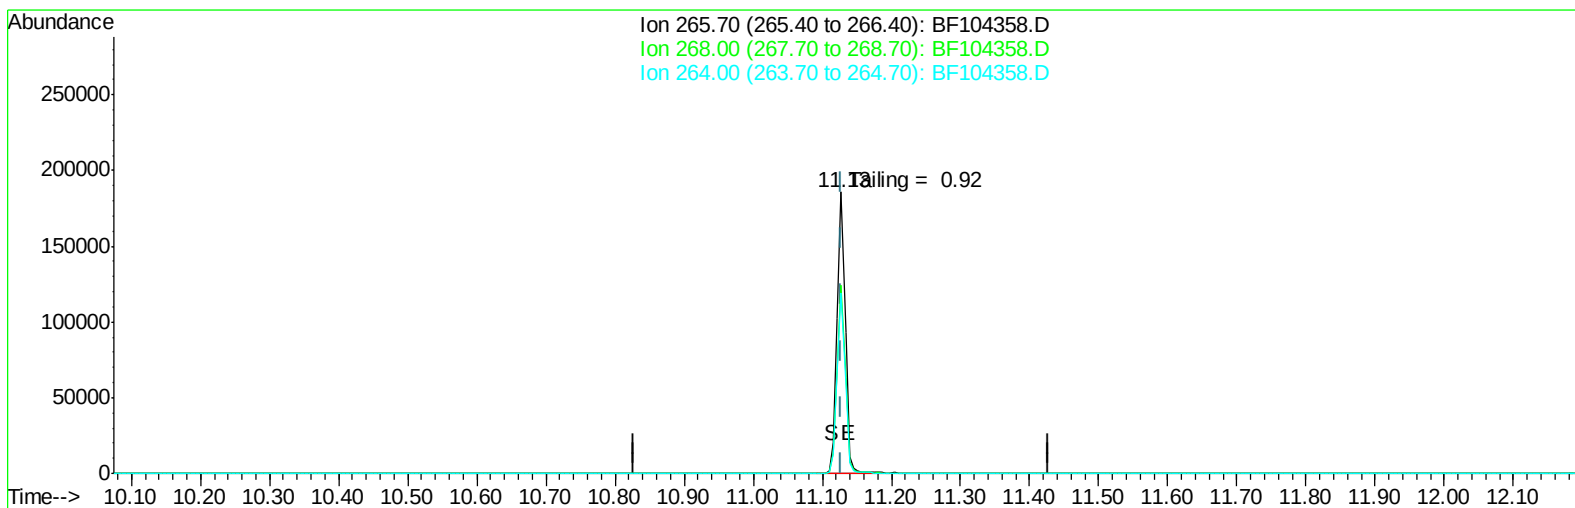

TIC: BF104358.D

(69) Pentachlorophenol (C)




11.127min (-0.000) 43111.07ng

response 149072

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.04
264.00	61.90	63.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040918\
Data File : BF104358.D
Acq On : 9 Apr 2018 8:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 04:18:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 06 16:44:53 2018
Response via : Initial Calibration

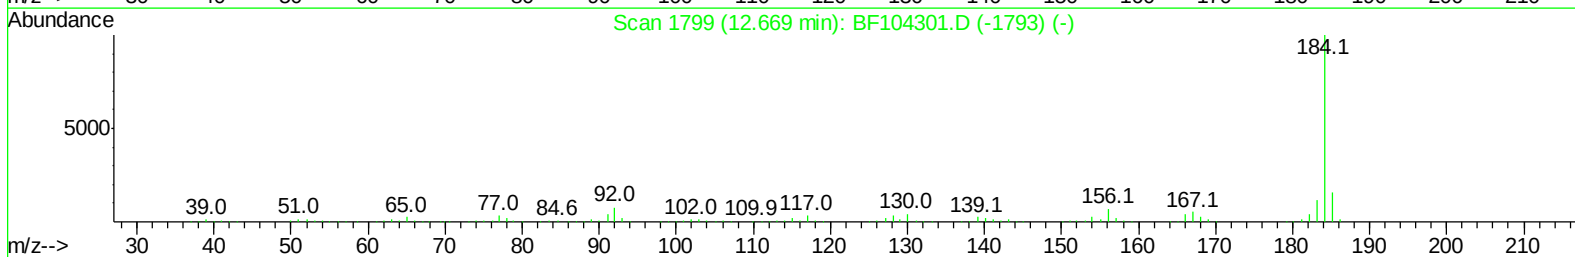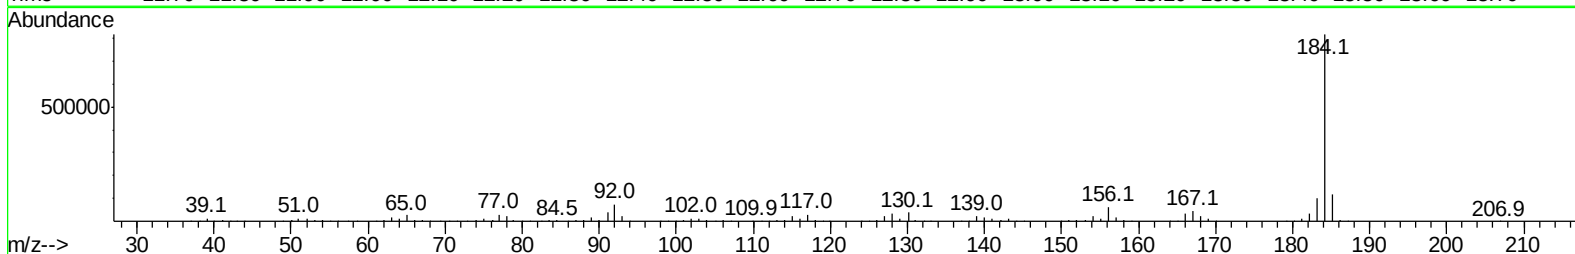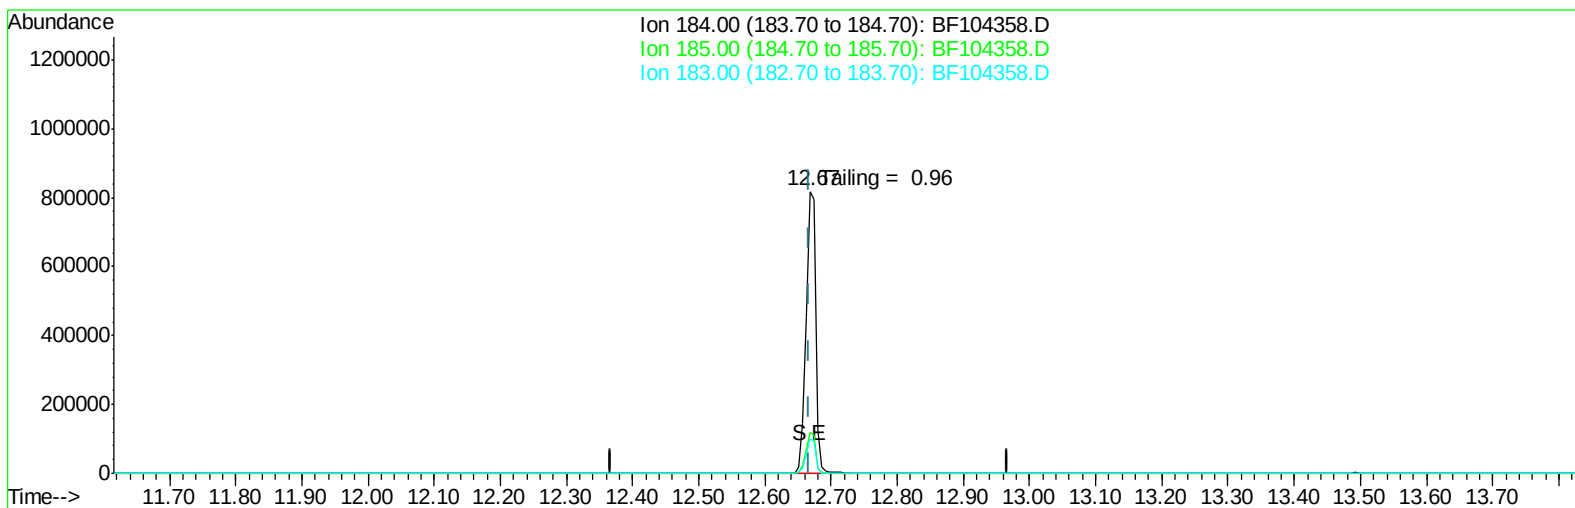

TIC: BF104358.D

(76) Benzidine

12.669min (+0.001) 0.00ng

response 852410

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.55
183.00	11.60	12.09
0.00	0.00	0.00