
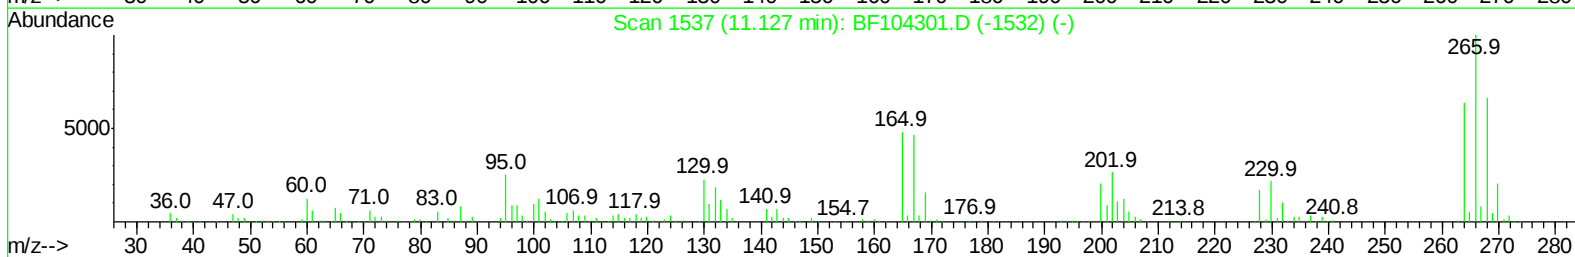
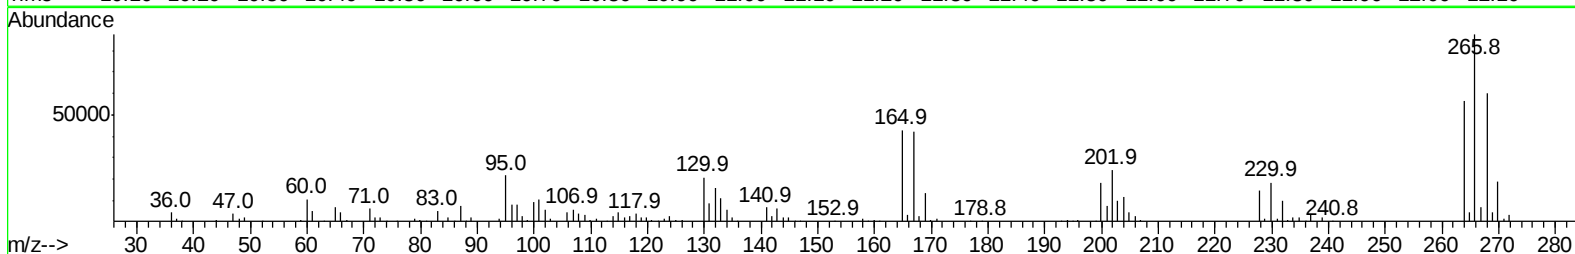


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040918\
Data File : BF104384.D
Acq On : 9 Apr 2018 21:29
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 04:20:45 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 06 16:44:53 2018
Response via : Initial Calibration

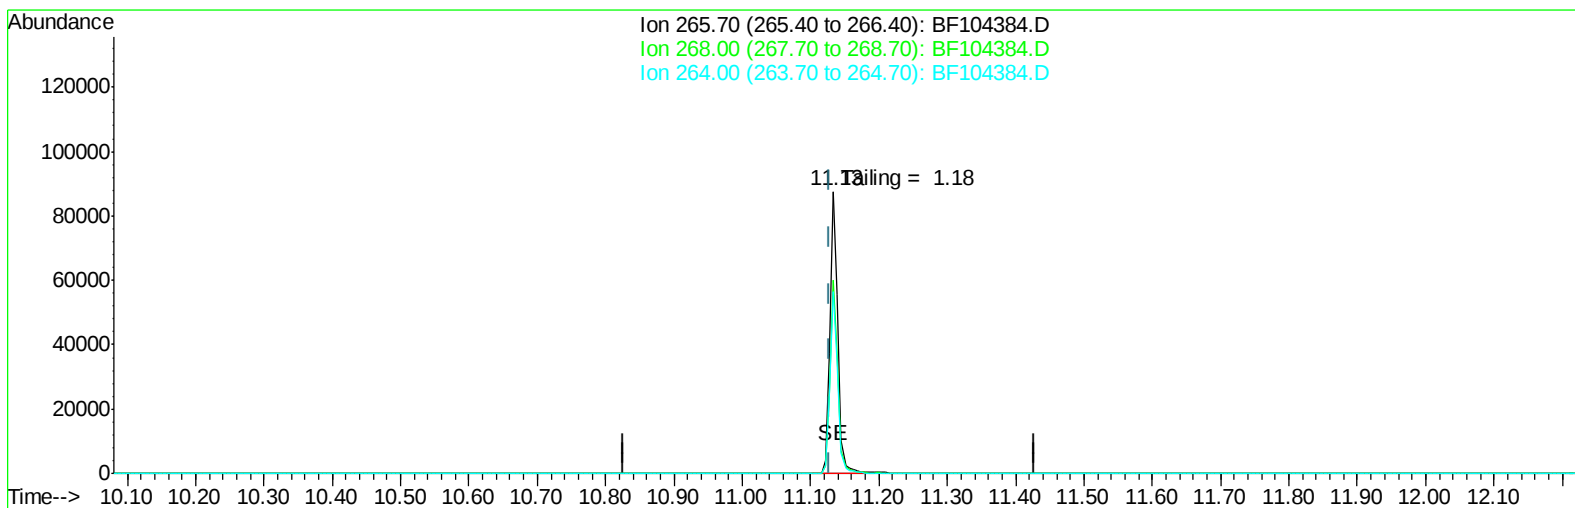

TIC: BF104384.D

(69) Pentachlorophenol (C)




11.133min (+0.006) 31372.46ng

response 71779

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.50
264.00	61.90	64.44
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040918\
 Data File : BF104384.D
 Acq On : 9 Apr 2018 21:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 04:20:45 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 06 16:44:53 2018
 Response via : Initial Calibration

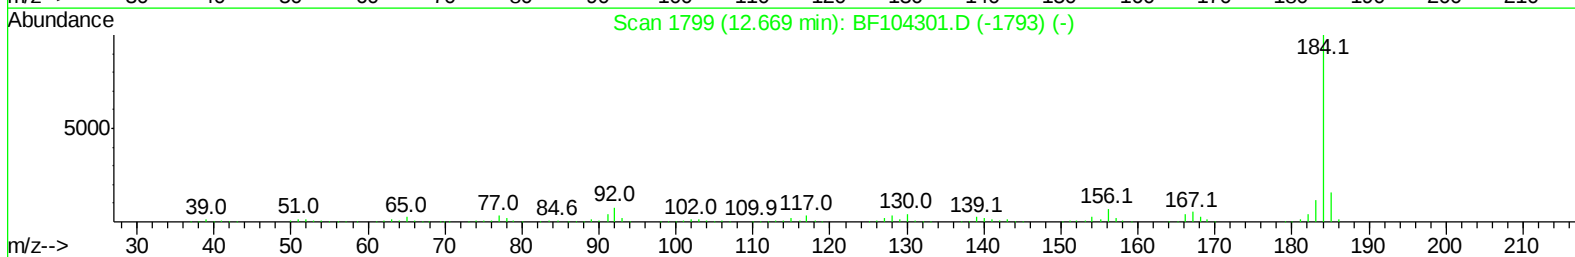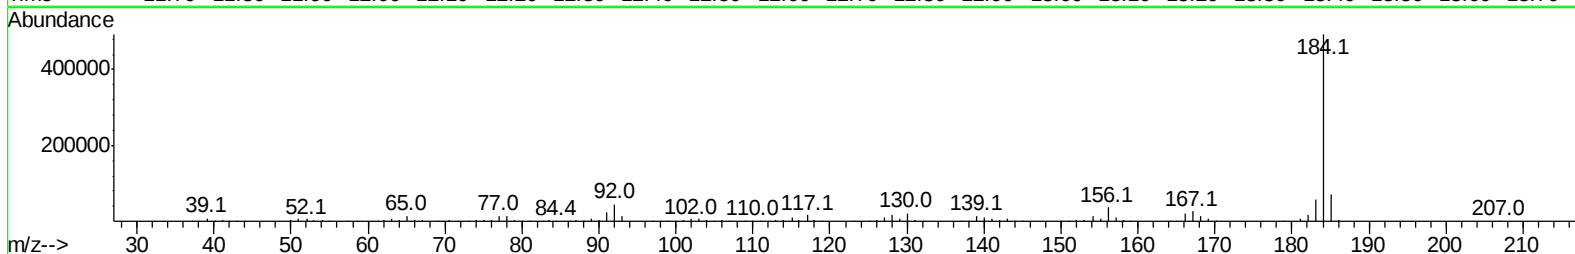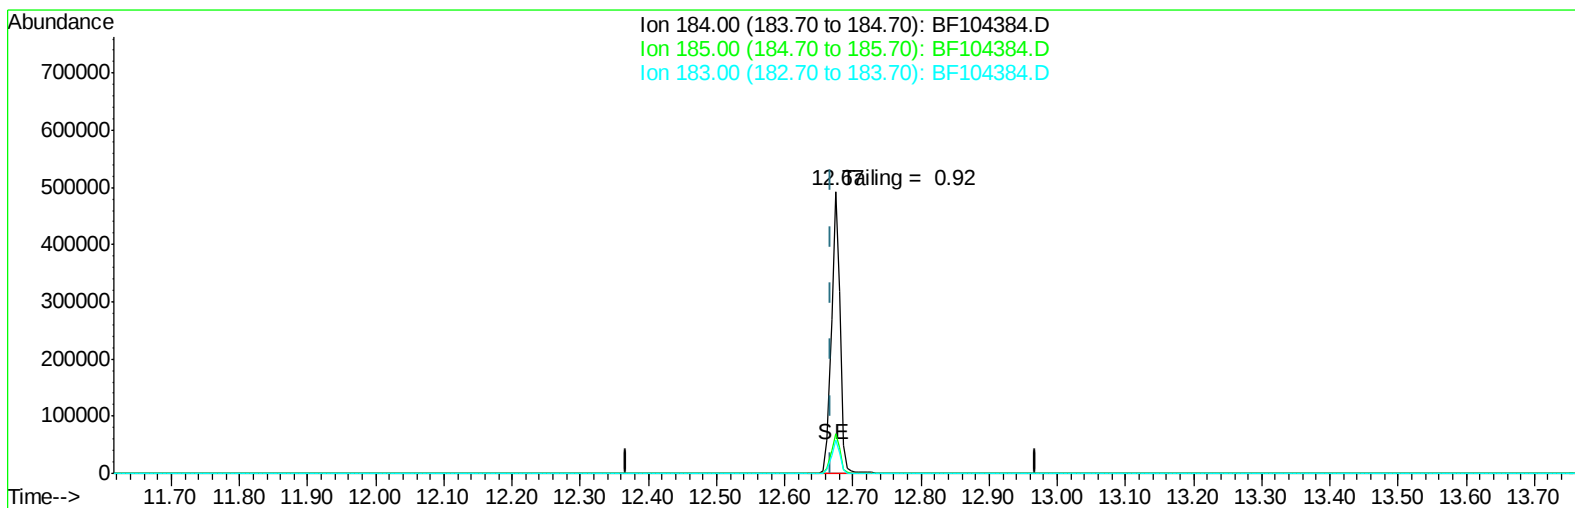

TIC: BF104384.D

(76) Benzidine

12.674min (+0.006) 0.00ng

response 431648

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.31
183.00	11.60	11.81
0.00	0.00	0.00