


Data Path : Z:\HPCHEM1\BNA F\Data\BF040918\
 Data File : BF104384.D
 Acq On : 9 Apr 2018 21:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 06 16:44:53 2018

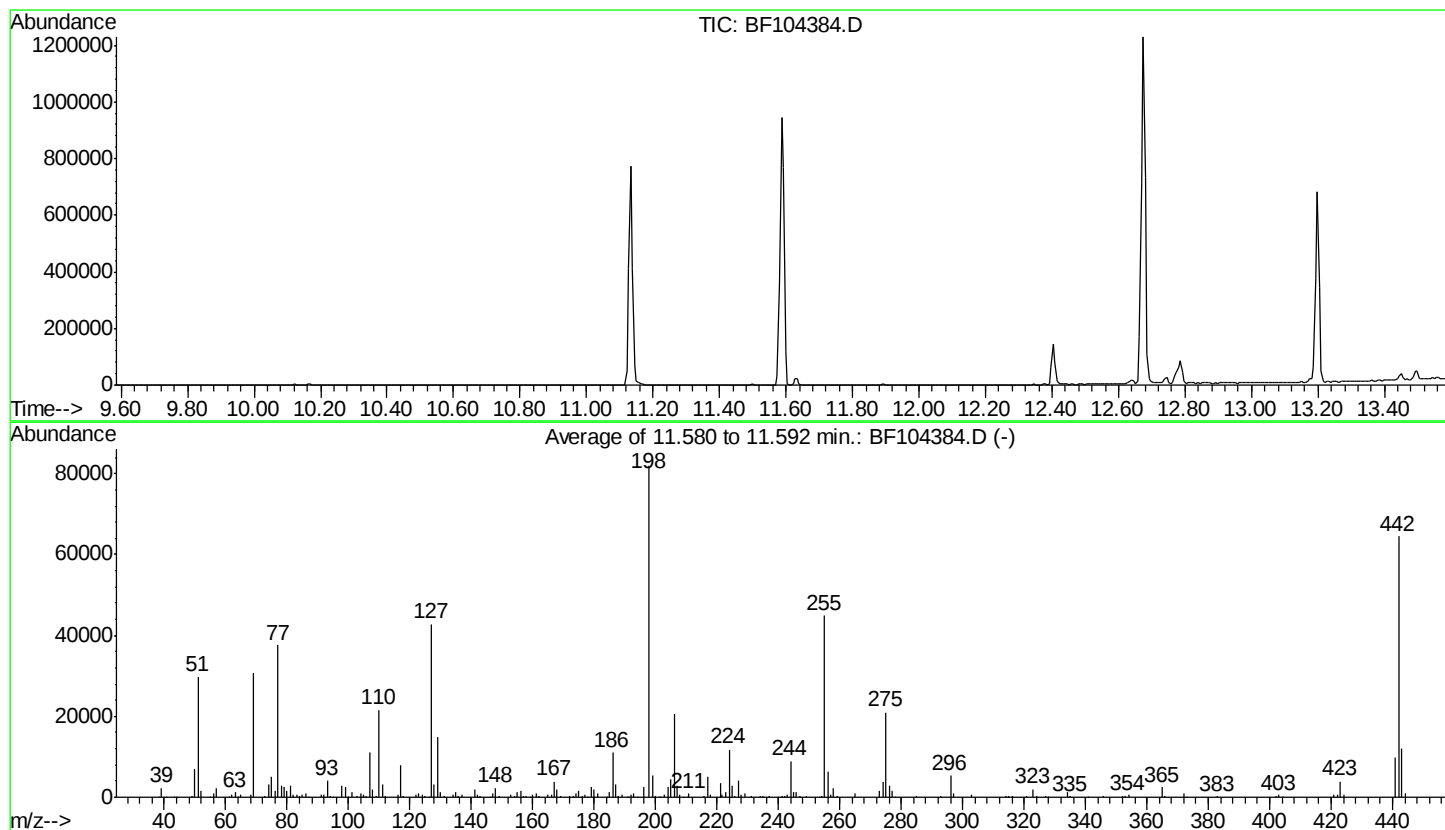

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	29850	PASS
68	69	0.00	2	1.8	538	PASS
69	198	0.00	100	37.3	30589	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	42786	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81976	PASS
199	198	5	9	6.6	5435	PASS
275	198	10	60	25.6	20981	PASS
365	198	1	100	2.9	2384	PASS
441	443	0.01	100	81.8	9922	PASS
442	198	50	100	78.6	64465	PASS
443	442	15	24	18.8	12127	PASS