

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040919\
 Data File : BF113657.D
 Acq On : 9 Apr 2019 13:13
 Operator : JU/SJ
 Sample : K2316-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 10 02:23:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	94418	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	358302	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	174657	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	368151	20.00	ng	-0.01
76) Chrysene-d12	13.83	240	356550	20.00	ng	-0.02
87) Perylene-d12	15.23	264	313417	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	695029	125.53	ng	0.00
7) Phenol-d6	6.33	99	907907	133.04	ng	0.00
23) Nitrobenzene-d5	7.25	82	516195	84.39	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	289319	137.90	ng	-0.01
45) 2-Fluorobiphenyl	9.03	172	883238	81.41	ng	-0.02
79) Terphenyl-d14	12.77	244	1036473	59.19	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.25	70	68278	16.225	ng	# 75
25) Isophorone	7.25	82	516189	43.806	ng	# 64
50) Dimethylphthalate	9.43	163	134793	10.470	ng	100
57) 2,4-Dinitrotoluene	9.71	165	22281	6.492	ng	# 23
67) 4-Bromophenyl-phenylether	10.50	248	16222	3.929	ng	# 1
84) Bis(2-ethylhexyl)phthalate	13.80	149	37554	2.813	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040919\
Data File : BF113657.D
Acq On : 9 Apr 2019 13:13
Operator : JU/SJ
Sample : K2316-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 10 02:23:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

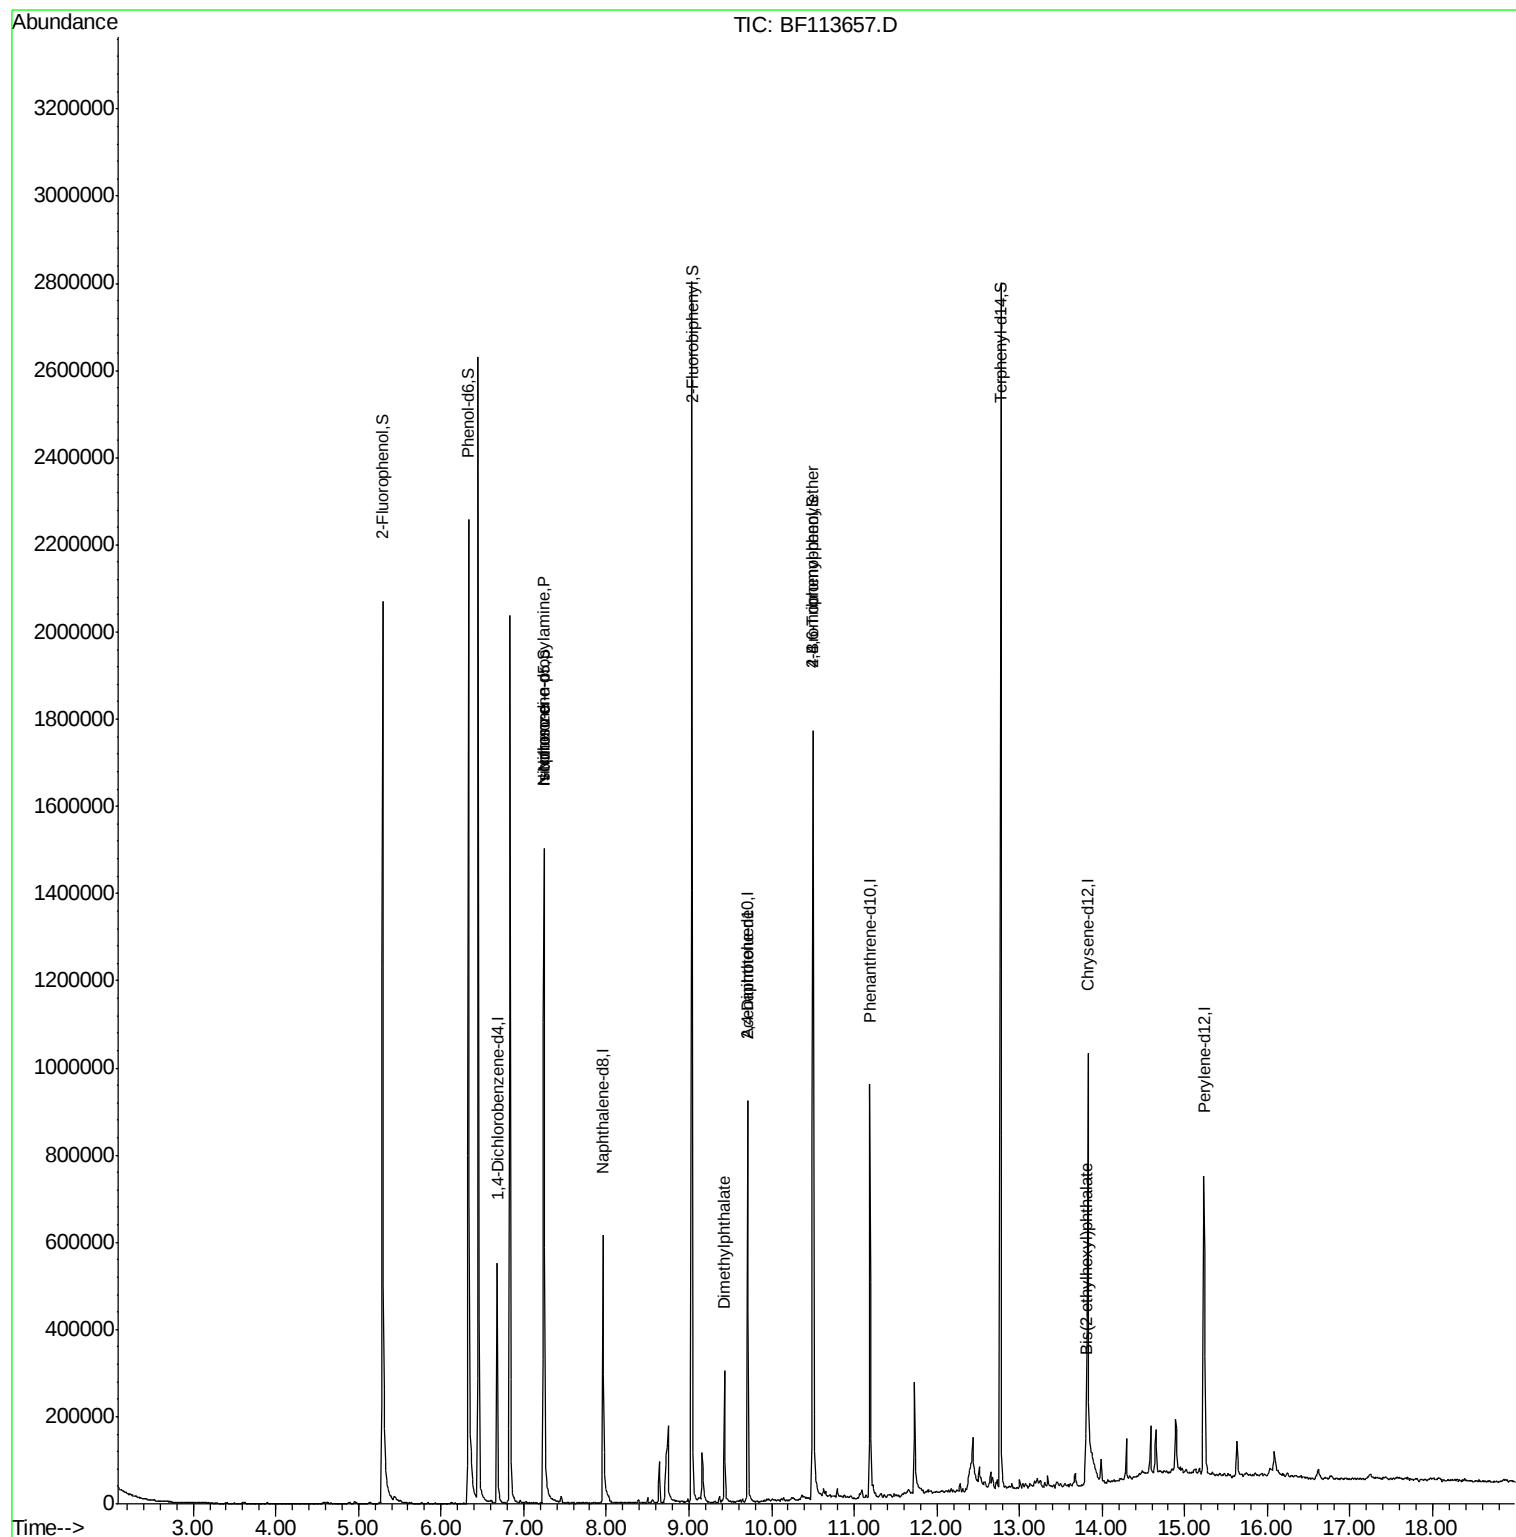




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.68 min Scan# 781
Delta R.T. -0.01 min
Lab File: BF113657.D
Acq: 9 Apr 2019 13:13

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 94418
Ion Ratio Lower Upper
152 100
150 155.1 124.7 187.1
115 55.1 46.0 69.0

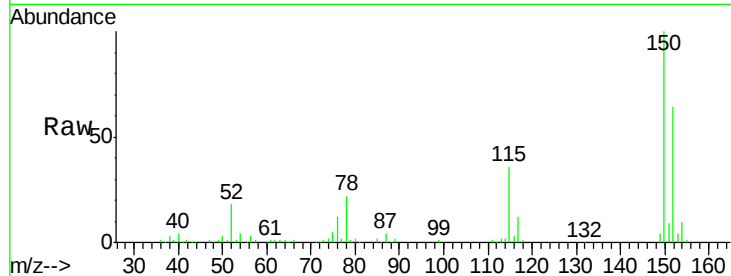


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

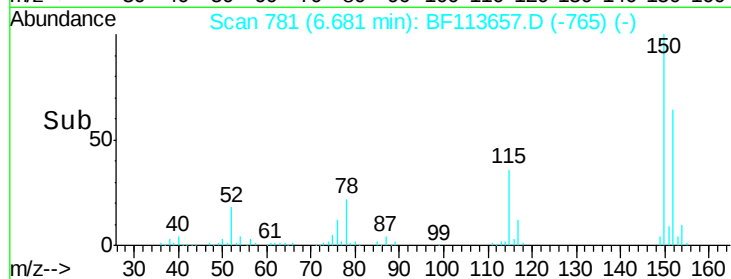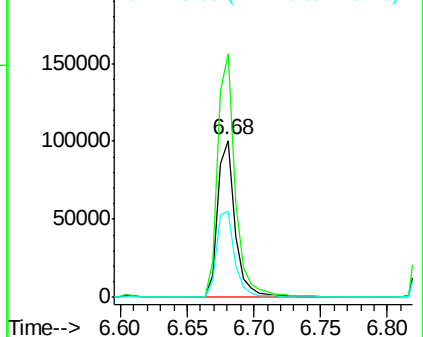



#5


2-Fluorophenol
Concen: 125.525 ng
RT: 5.29 min Scan# 545
Delta R.T. -0.01 min
Lab File: BF113657.D
Acq: 9 Apr 2019 13:13

Tgt Ion:112 Resp: 695029
Ion Ratio Lower Upper
112 100
64 59.3 49.2 73.8
63 30.0 24.9 37.3

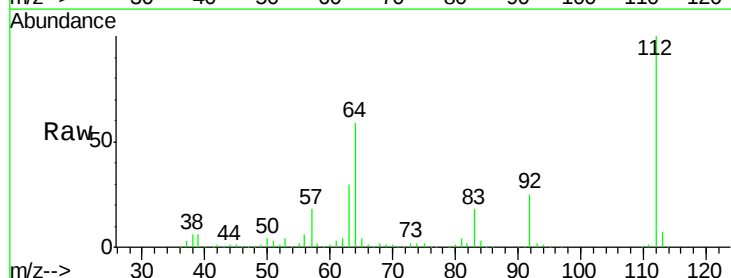

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

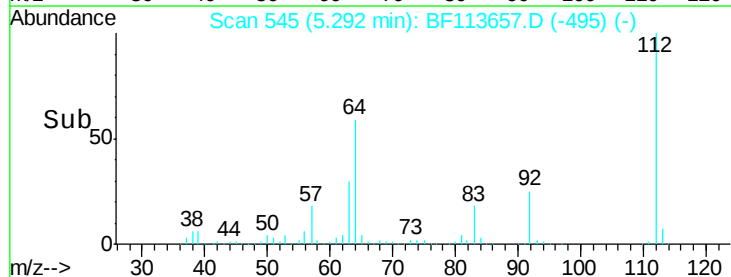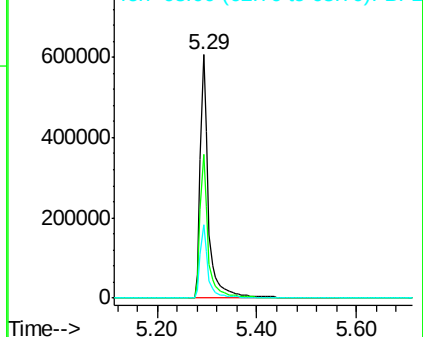

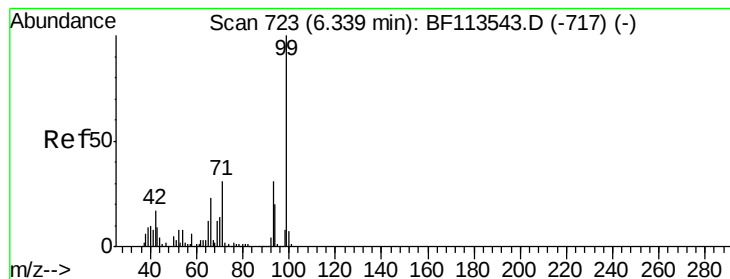

#7

Phenol-d6

Concen: 133.039 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 907907

Ion Ratio Lower Upper

99 100

42 17.2 14.8 22.2

71 31.1 24.9 37.3

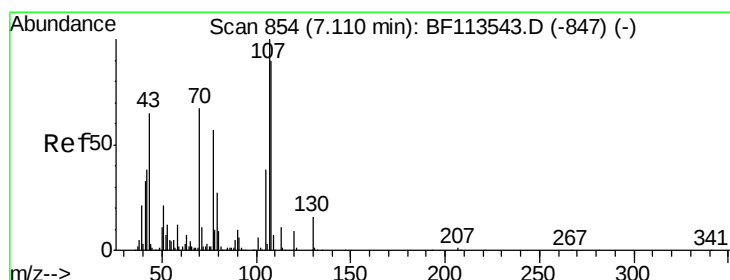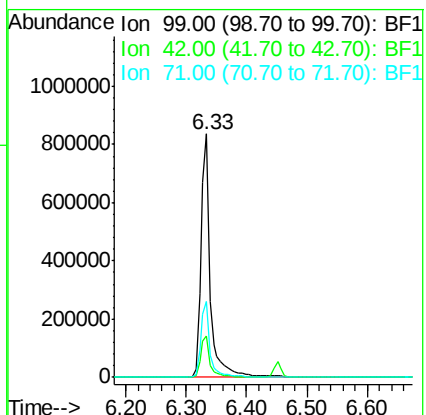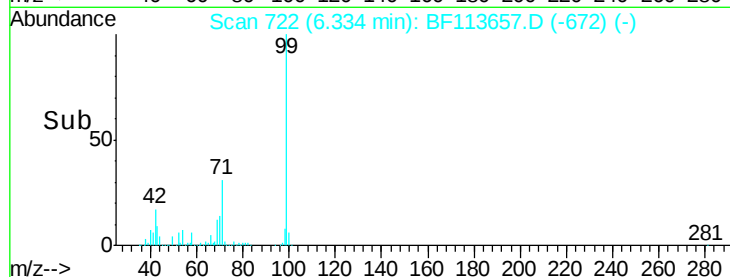

#19

n-Nitroso-di-n-propylamine

Concen: 16.225 ng

RT: 7.25 min Scan# 877

Delta R.T. 0.14 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13

Tgt Ion: 70 Resp: 68278




Ion Ratio Lower Upper

70 100

42 47.1 48.4 72.6#

101 0.0 7.8 11.8#

130 2.5 18.2 27.4#

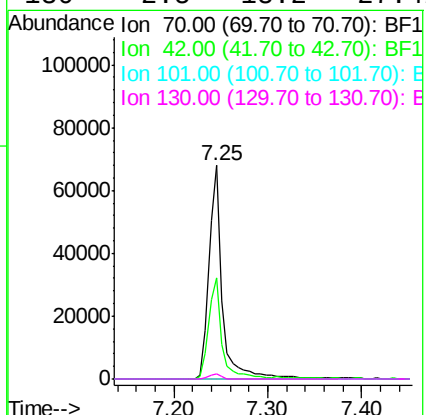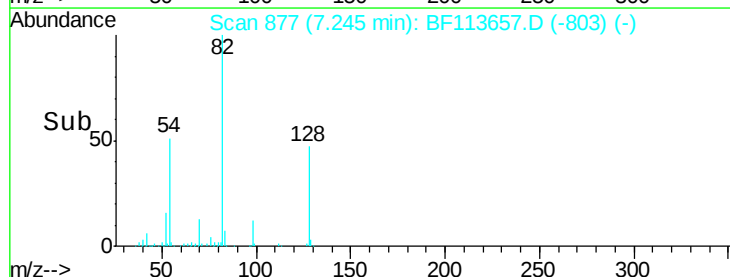



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13

Instrument :

BNA_F

ClientSampled :

Tot Ion:136 Resp: 358302


Ion Ratio Lower Upper

136 100

137 10.4 8.9 13.3

54 7.4 7.0 10.6

68 5.6 4.8 7.2


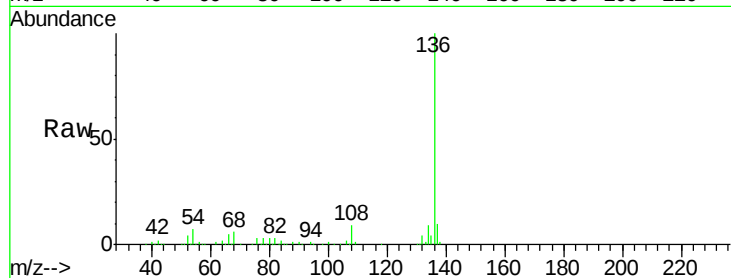


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

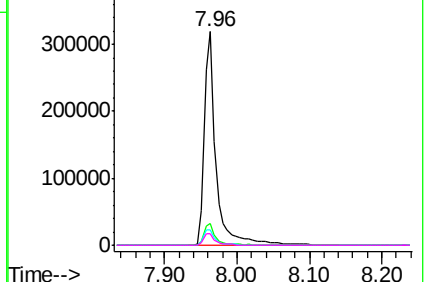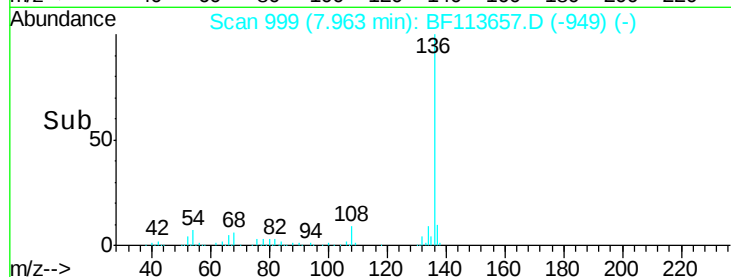

#23

Nitrobenzene-d5

Concen: 84.388 ng

RT: 7.25 min Scan# 877

Delta R.T. -0.01 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13


Tgt Ion: 82 Resp: 516195

Ion Ratio Lower Upper

82 100

128 46.9 36.5 54.7



54 50.9 42.2 63.2

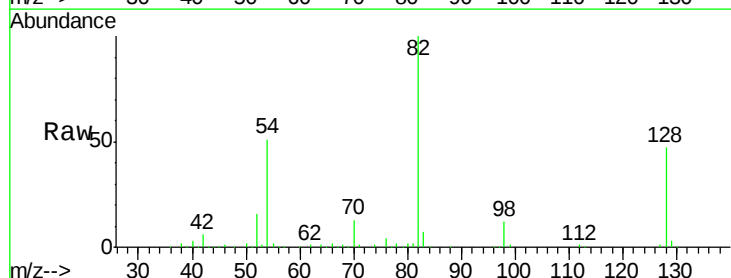

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

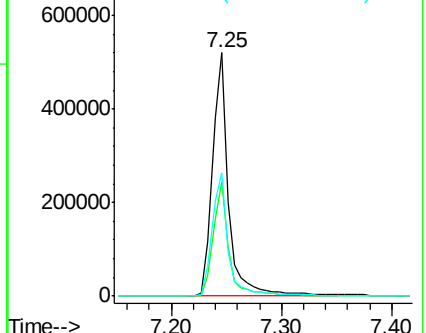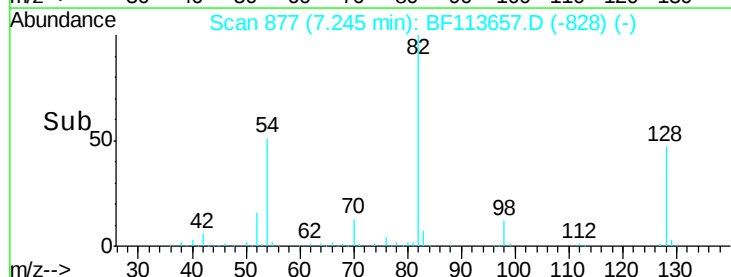



#25

Isophorone

Concen: 43.806 ng

RT: 7.25 min Scan# 877

Delta R.T. -0.27 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 82 Resp: 516189

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#

138 0.0 15.2 22.8#

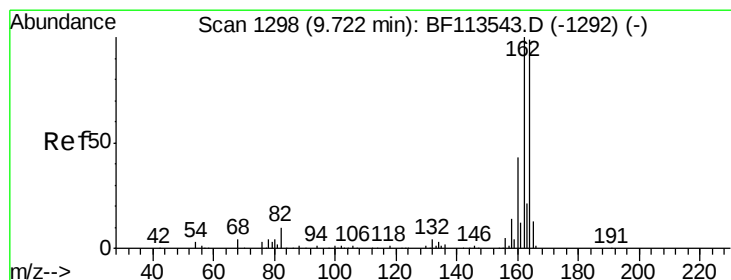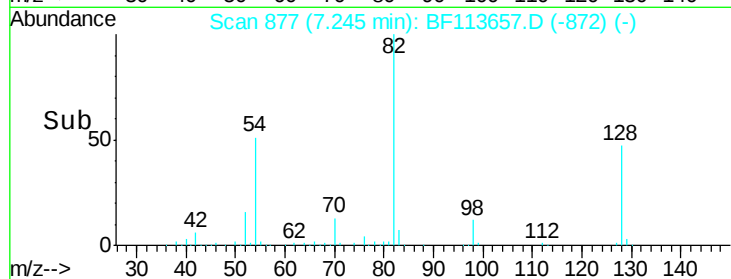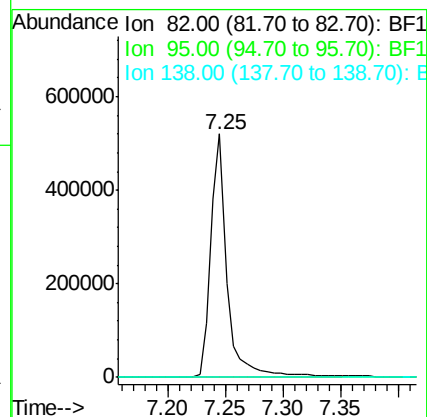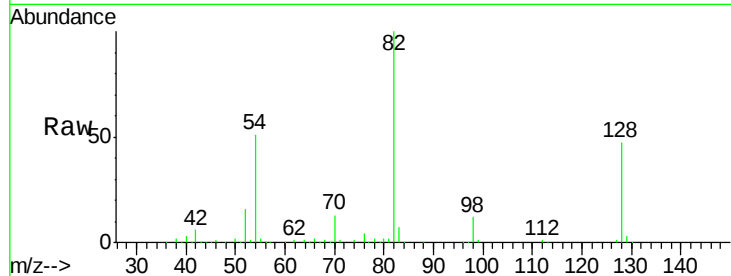

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.71 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13




Tgt Ion:164 Resp: 174657

Ion Ratio Lower Upper

164 100

162 102.3 81.8 122.6

160 45.0 36.4 54.6

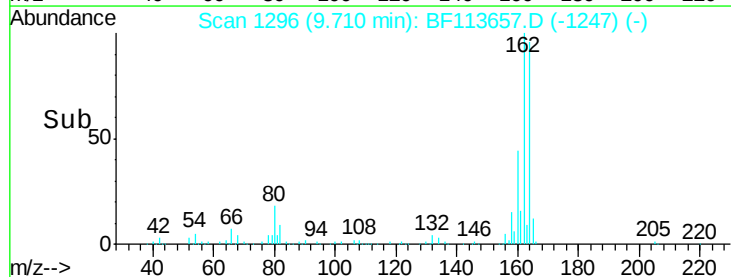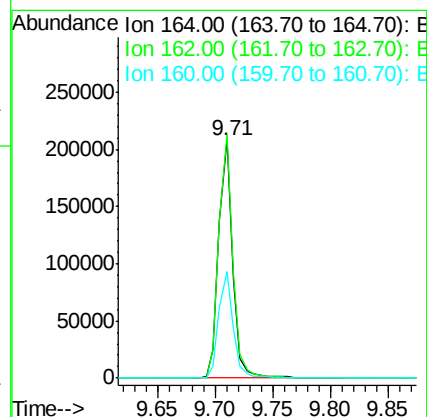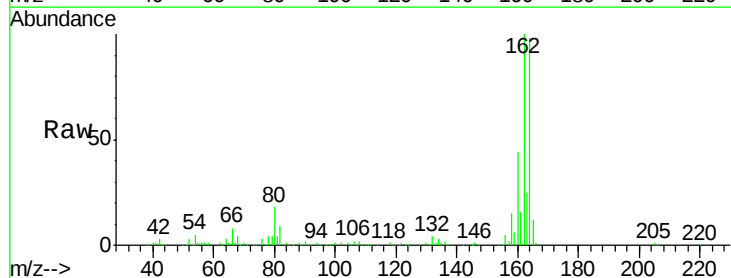



#42

2,4,6-Tribromophenol

Concen: 137.899 ng

RT: 10.50 min Scan# 1431

Delta R.T. -0.01 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13

Instrument :

BNA_F

ClientSampleId :


Tot Ion:330 Resp: 289319

Ion Ratio Lower Upper

330 100

332 96.2 77.8 116.6




141 27.5 22.7 34.1

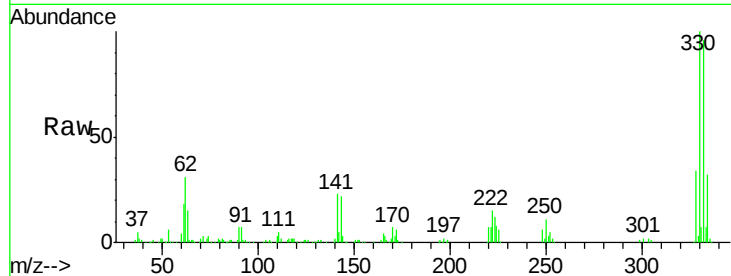

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

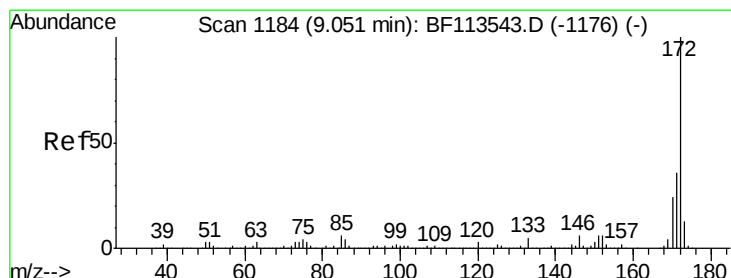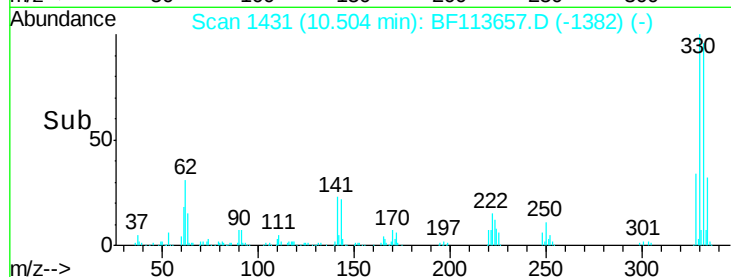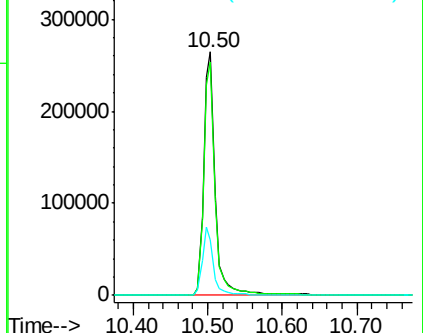

#45

2-Fluorobiphenyl

Concen: 81.412 ng

RT: 9.03 min Scan# 1181

Delta R.T. -0.02 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13


Tgt Ion:172 Resp: 883238

Ion Ratio Lower Upper

172 100

171 35.4 29.0 43.6



170 23.8 19.5 29.3

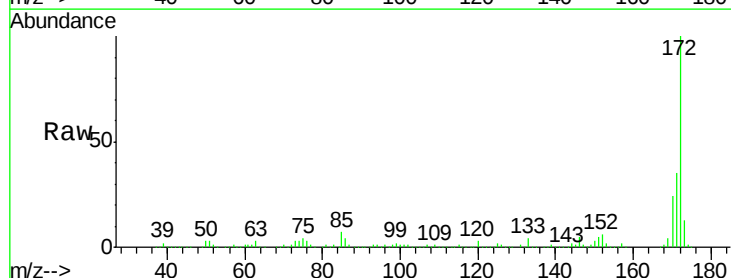

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

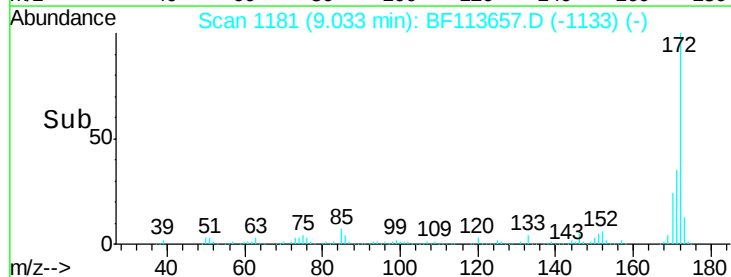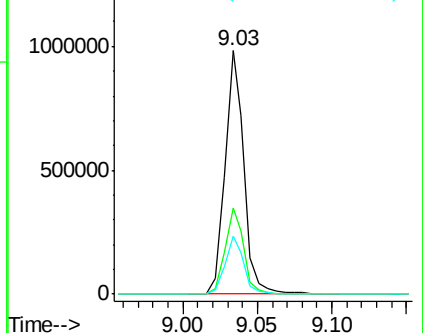







#50
Dimethylphthalate
Concen: 10.470 ng
RT: 9.43 min Scan# 1248
Delta R.T. -0.02 min
Lab File: BF113657.D
Acq: 9 Apr 2019 13:13

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.0	4.6
164	10.2	8.1	12.1

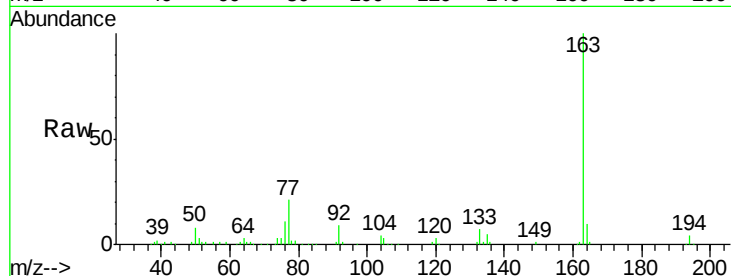


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

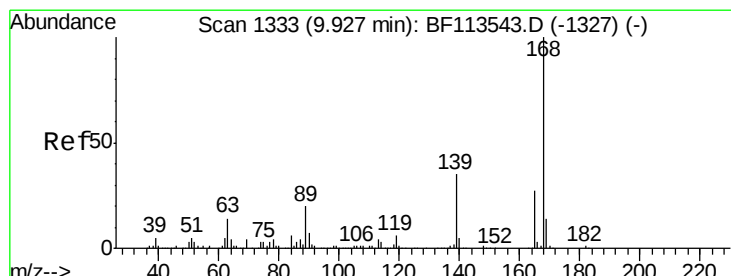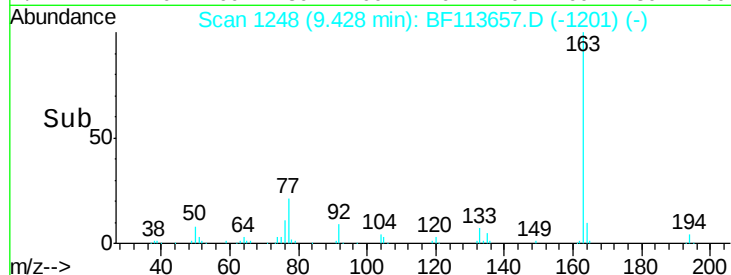
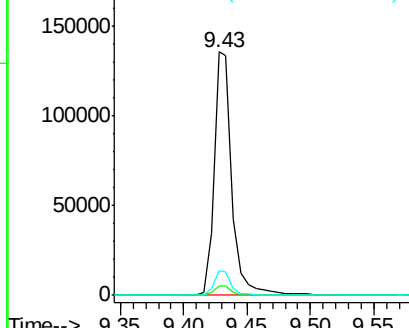



#57
2,4-Dinitrotoluene
Concen: 6.492 ng
RT: 9.71 min Scan# 1296
Delta R.T. -0.22 min
Lab File: BF113657.D
Acq: 9 Apr 2019 13:13

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.4	37.5	56.3#
89	1.6	57.4	86.2#
182	0.0	2.0	3.0#

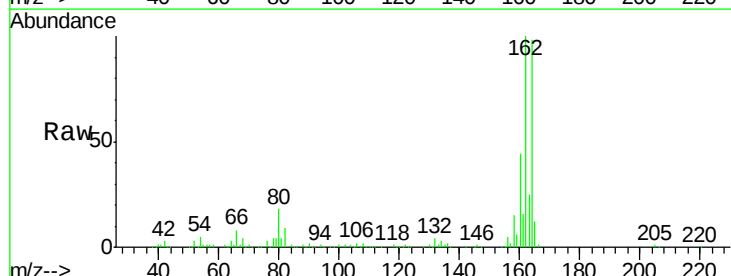

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): E



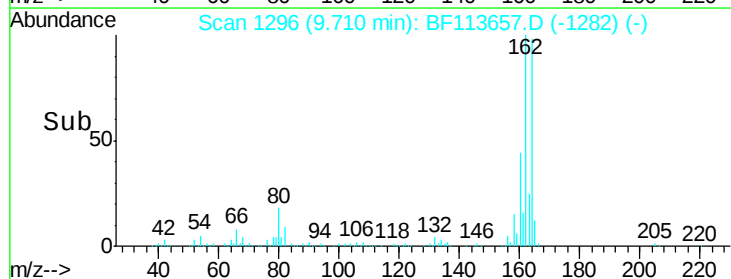
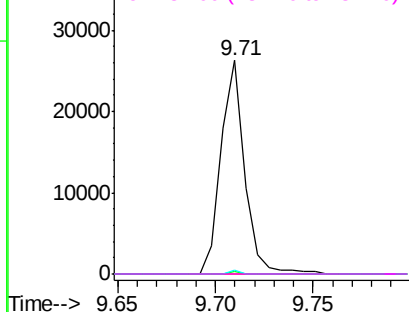


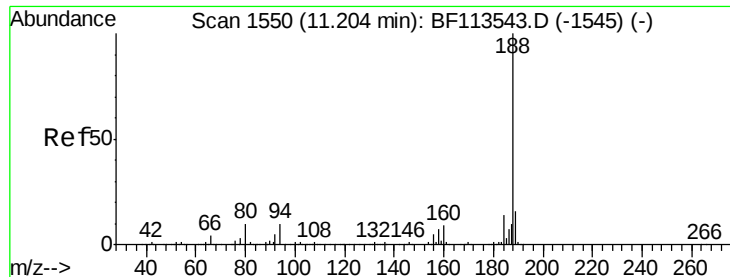

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.19 min Scan# 1548
 Delta R.T. -0.01 min
 Lab File: BF113657.D
 Acq: 9 Apr 2019 13:13




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:188 Resp: 368151
 Ion Ratio Lower Upper
 188 100
 94 9.2 7.0 10.6
 80 9.2 7.7 11.5

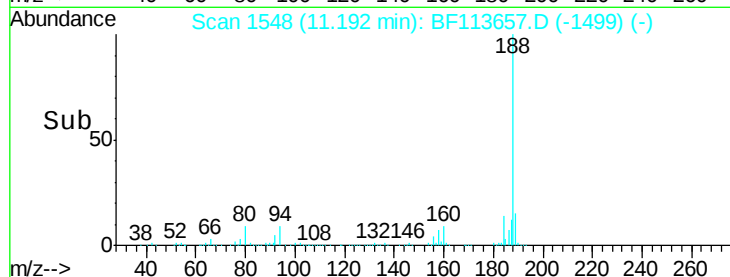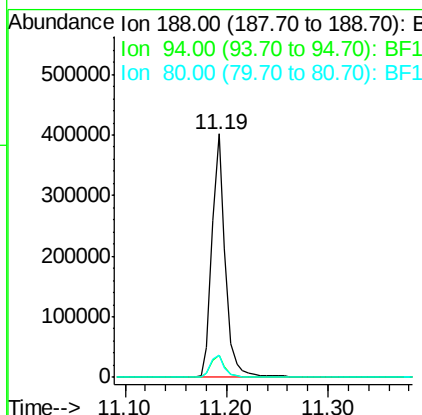

#67
 4-Bromophenyl-phenylether
 Concen: 3.929 ng
 RT: 10.50 min Scan# 1430
 Delta R.T. -0.25 min
 Lab File: BF113657.D
 Acq: 9 Apr 2019 13:13

Tgt Ion:248 Resp: 16222
 Ion Ratio Lower Upper
 248 100
 250 186.4 78.3 117.5#
 141 495.7 56.2 84.4#

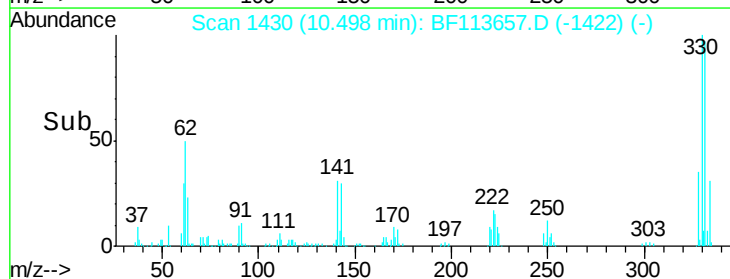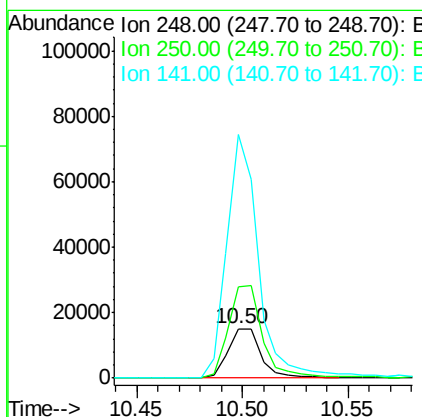

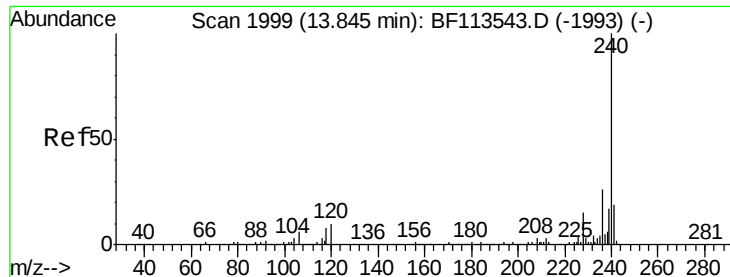

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1996

Delta R.T. -0.02 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 356550

Ion Ratio Lower Upper

240 100

120 10.0 8.8 13.2




236 24.8 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

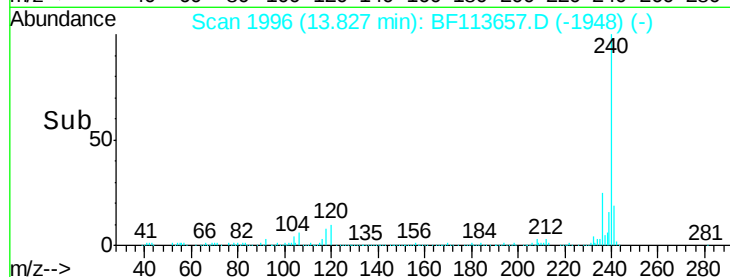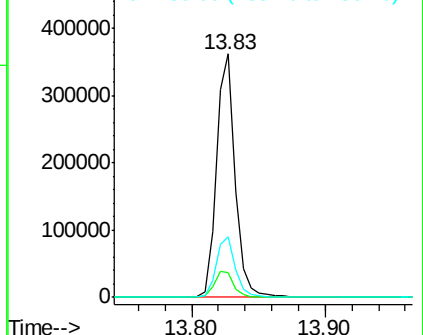

#79

Terphenyl-d14

Concen: 59.186 ng

RT: 12.77 min Scan# 1817

Delta R.T. -0.02 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13


Tgt Ion:244 Resp: 1036473

Ion Ratio Lower Upper

244 100

212 6.5 5.5 8.3



122 9.9 8.6 13.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

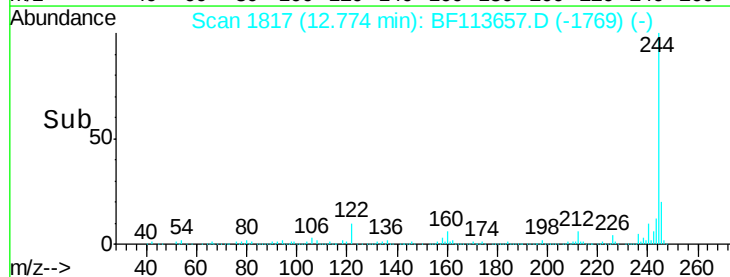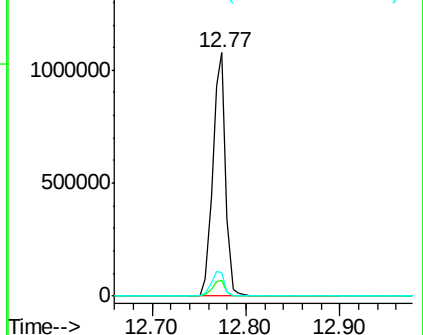

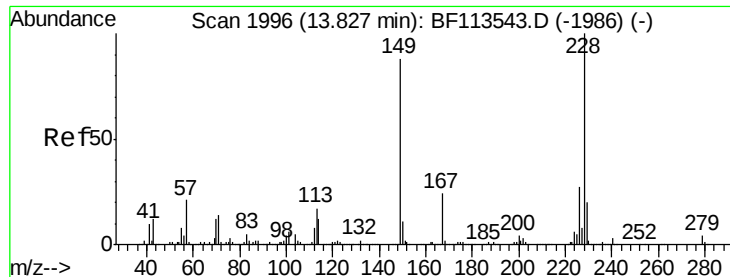

#84

Bis(2-ethylhexyl)phthalate

Concen: 2.813 ng

RT: 13.80 min Scan# 1992

Delta R.T. -0.02 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13

Instrument :

BNA_F

ClientSampleId :


Tot Ion:149 Resp: 37554

Ion Ratio Lower Upper

149 100

167 27.7 21.8 32.8




279 4.1 2.9 4.3



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

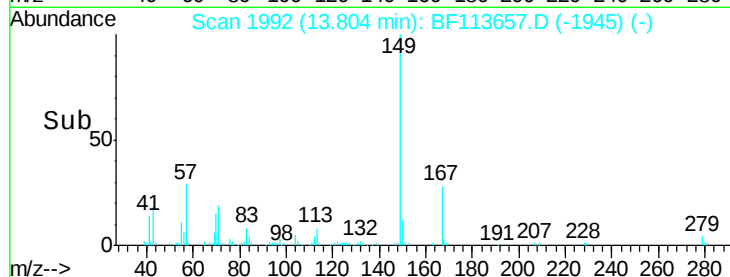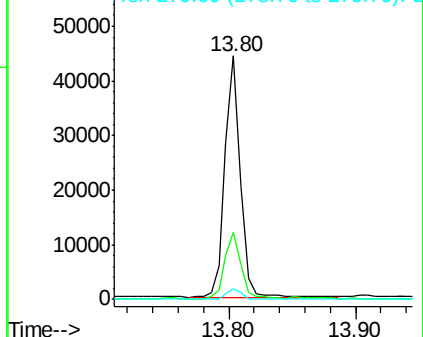

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.23 min Scan# 2235

Delta R.T. -0.02 min

Lab File: BF113657.D

Acq: 9 Apr 2019 13:13


Tgt Ion:264 Resp: 313417

Ion Ratio Lower Upper

264 100

260 23.5 19.1 28.7

265 21.8 17.1 25.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

