

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040919\
 Data File : BF113679.D
 Acq On : 10 Apr 2019 2:04
 Operator : JU/SJ
 Sample : K2338-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 10 04:57:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	98771	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	368369	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	169611	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	311316	20.00	ng	-0.01
76) Chrysene-d12	13.83	240	259043	20.00	ng	-0.02
87) Perylene-d12	15.23	264	257996	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	692889	119.62	ng	0.00
7) Phenol-d6	6.33	99	809831	113.44	ng	-0.01
23) Nitrobenzene-d5	7.25	82	600570	95.50	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	283744	139.26	ng	-0.02
45) 2-Fluorobiphenyl	9.03	172	1107385	105.11	ng	-0.02
79) Terphenyl-d14	12.77	244	1065900	83.78	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.25	70	77318	17.564	ng	# 75
25) Isophorone	7.25	82	601478	49.649	ng	# 64
50) Dimethylphthalate	9.71	163	40266	3.221	ng	# 1
51) 2,6-Dinitrotoluene	9.71	165	21138	7.670	ng	# 25
57) 2,4-Dinitrotoluene	9.71	165	21138	6.342	ng	# 22
67) 4-Bromophenyl-phenylether	10.50	248	14522	4.159	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040919\
Data File : BF113679.D
Acq On : 10 Apr 2019 2:04
Operator : JU/SJ
Sample : K2338-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 10 04:57:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

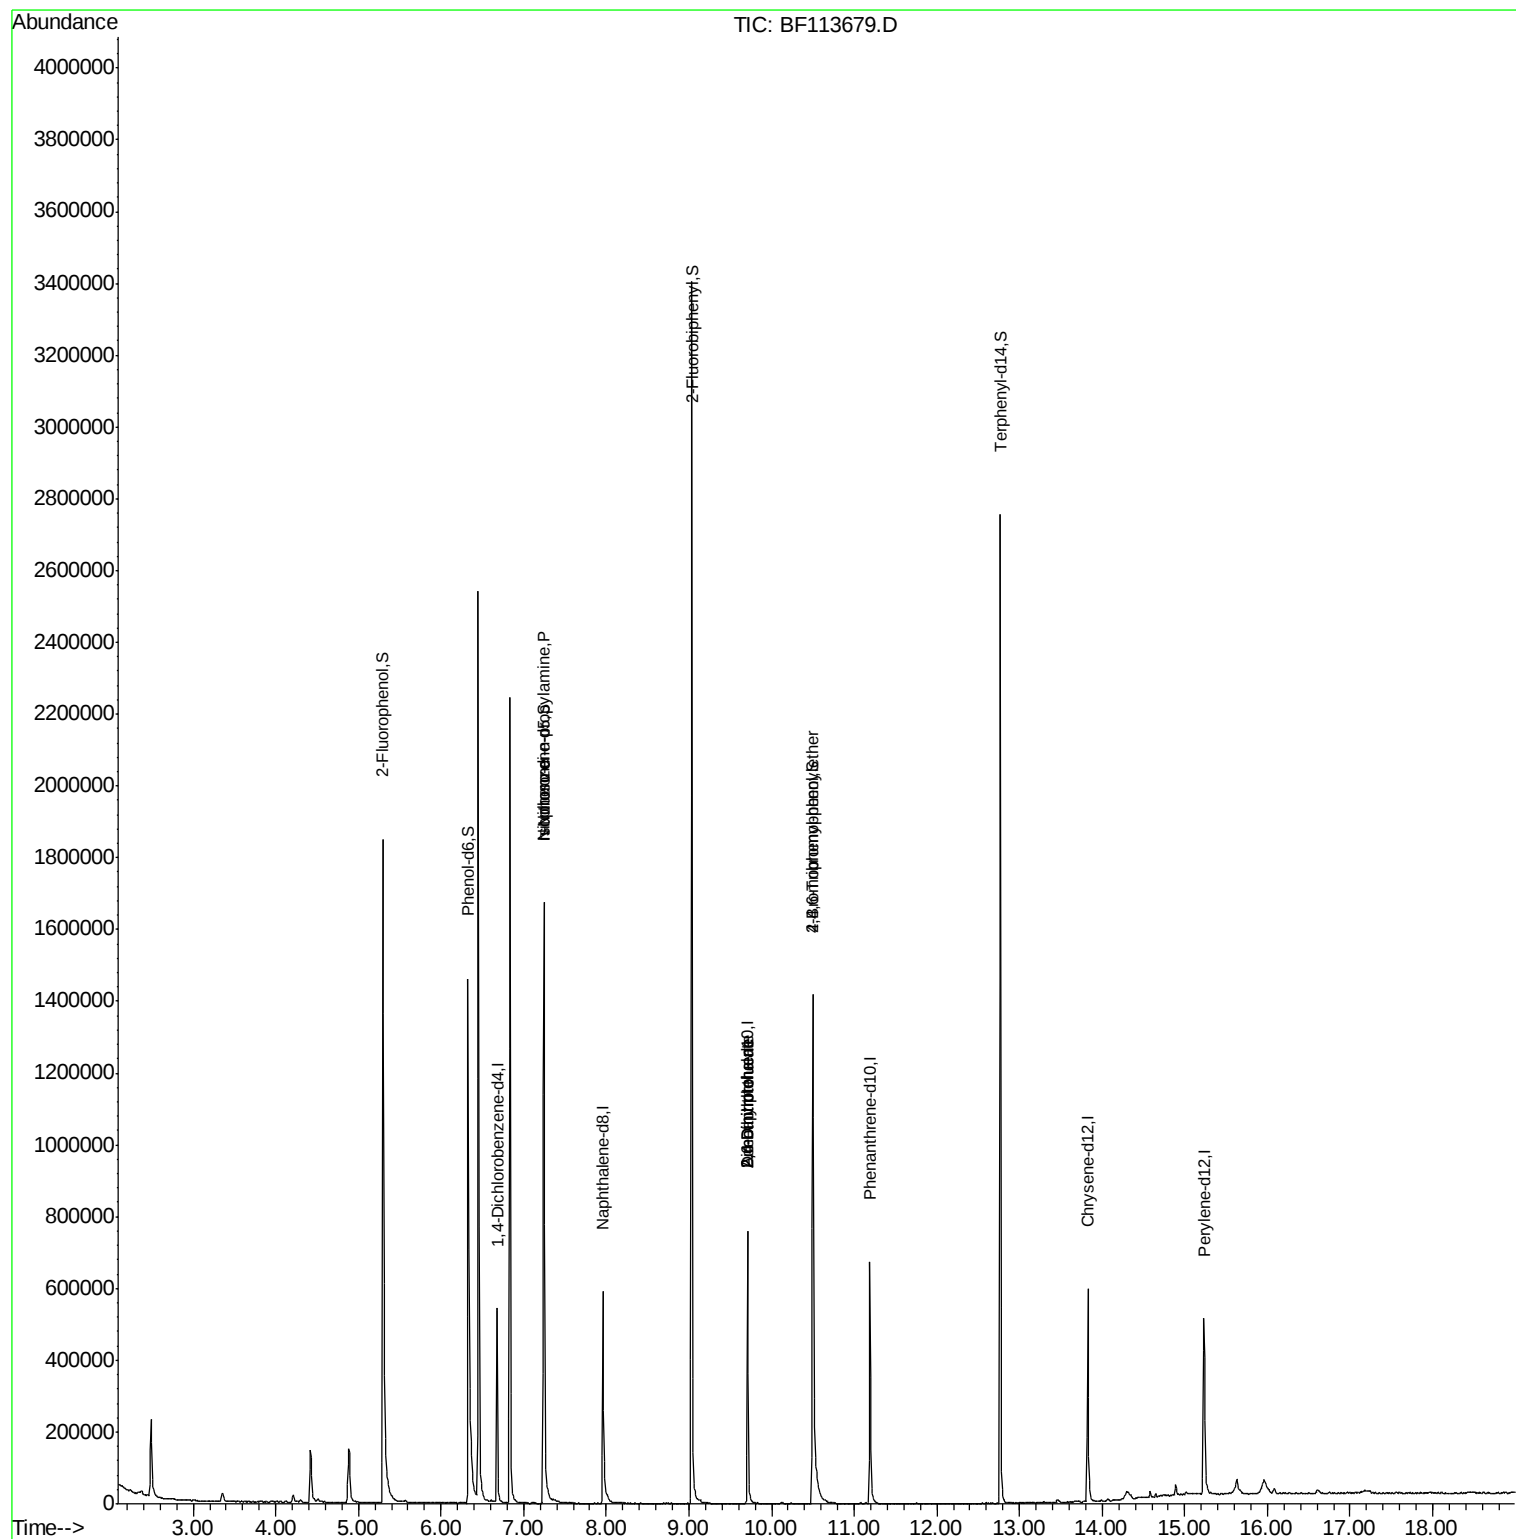




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.68 min Scan# 781
 Delta R.T. -0.01 min
 Lab File: BF113679.D
 Acq: 10 Apr 2019 2:04

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 98771
 Ion Ratio Lower Upper
 152 100
 150 157.7 124.7 187.1
 115 53.5 46.0 69.0

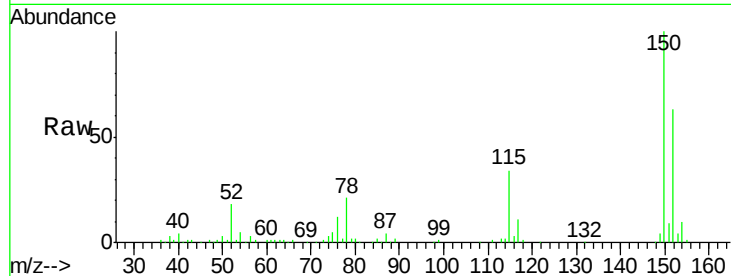


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

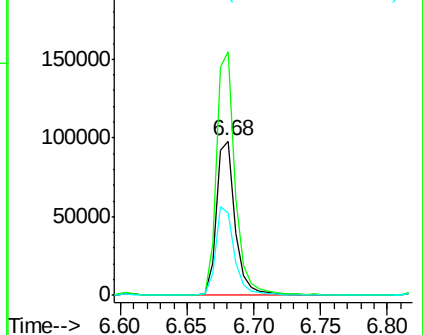



#5


2-Fluorophenol
 Concen: 119.624 ng
 RT: 5.30 min Scan# 546
 Delta R.T. 0.00 min
 Lab File: BF113679.D
 Acq: 10 Apr 2019 2:04

Tgt Ion:112 Resp: 692889
 Ion Ratio Lower Upper
 112 100
 64 59.8 49.2 73.8
 63 29.7 24.9 37.3

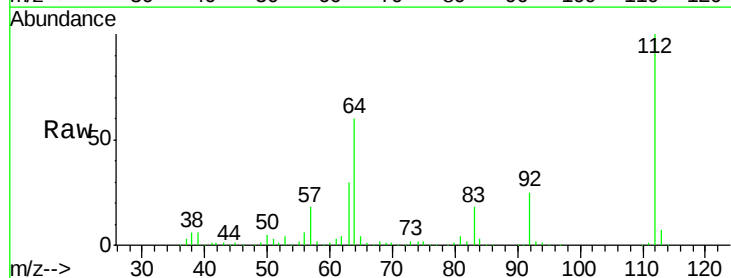

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

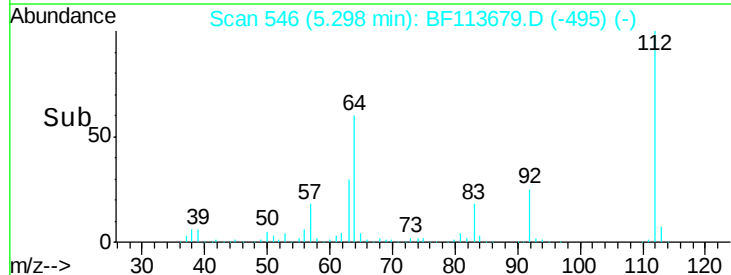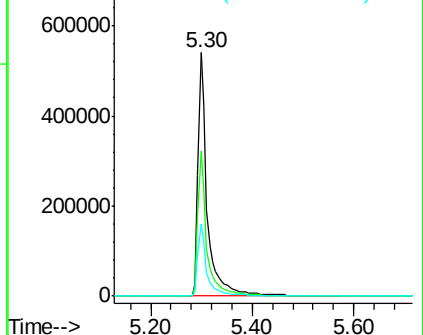

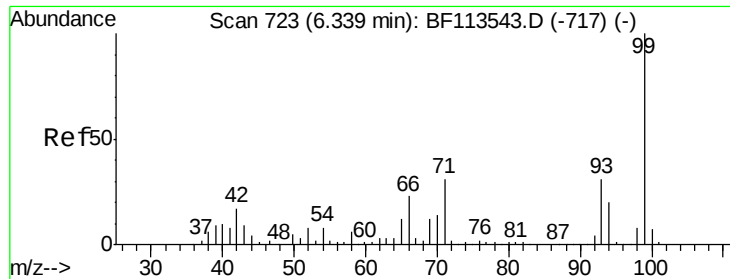

#7

Phenol-d6

Concen: 113.438 ng

RT: 6.33 min Scan# 721

Delta R.T. -0.01 min

Lab File: BF113679.D

Acq: 10 Apr 2019 2:04

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 809831

Ion Ratio Lower Upper

99 100

42 18.5 14.8 22.2




71 31.4 24.9 37.3

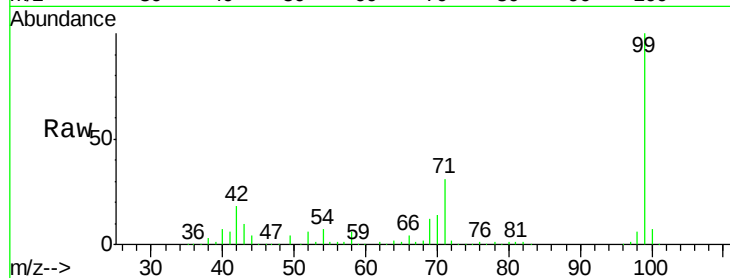

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

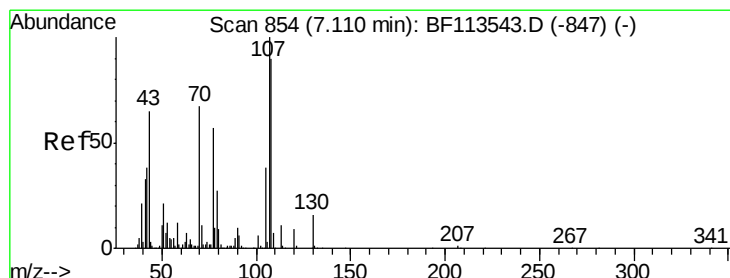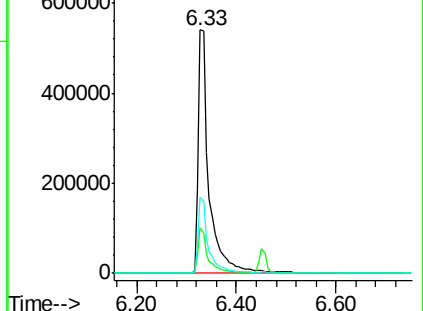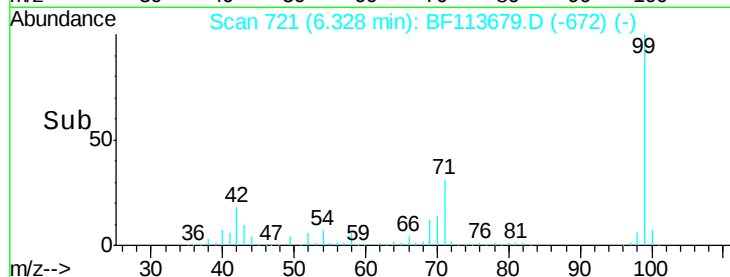

#19

n-Nitroso-di-n-propylamine

Concen: 17.564 ng

RT: 7.25 min Scan# 877

Delta R.T. 0.14 min

Lab File: BF113679.D

Acq: 10 Apr 2019 2:04

Tgt Ion: 70 Resp: 77318


Ion Ratio Lower Upper

70 100

42 46.6 48.4 72.6#

101 0.0 7.8 11.8#

130 2.2 18.2 27.4#


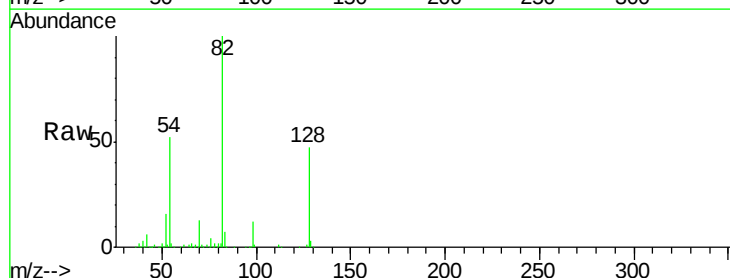


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

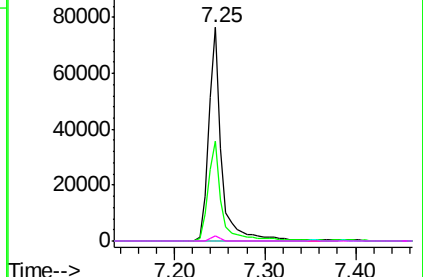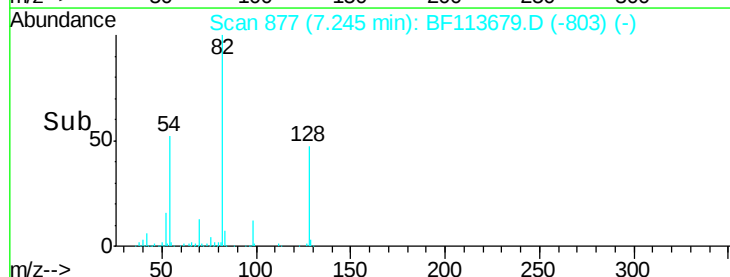







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.96 min Scan# 999
Delta R.T. -0.01 min
Lab File: BF113679.D
Acq: 10 Apr 2019 2:04

Instrument :
BNA_F
ClientSampled :

Tot Ion:136	Resp:	368369
Ion	Ratio	Lower Upper
136	100	
137	10.5	8.9 13.3
54	7.4	7.0 10.6
68	5.3	4.8 7.2

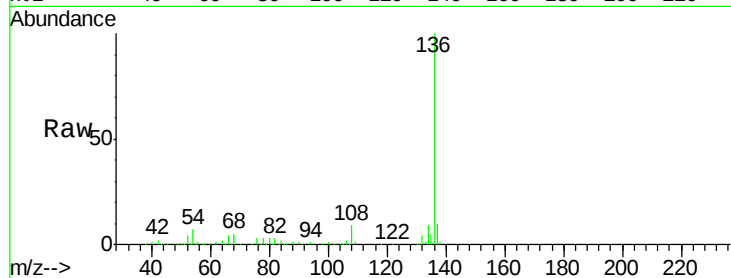


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

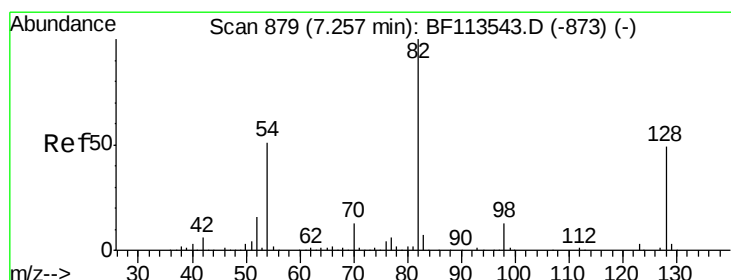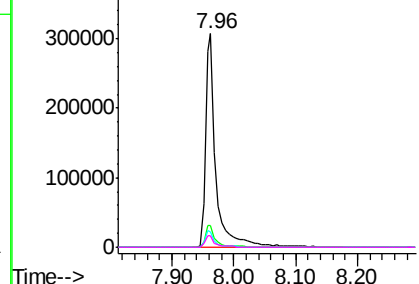




#23
Nitrobenzene-d5
Concen: 95.498 ng
RT: 7.25 min Scan# 877
Delta R.T. -0.01 min
Lab File: BF113679.D
Acq: 10 Apr 2019 2:04

Tgt Ion: 82	Resp:	600570
Ion	Ratio	Lower Upper
82	100	
128	47.3	36.5 54.7
54	51.8	42.2 63.2

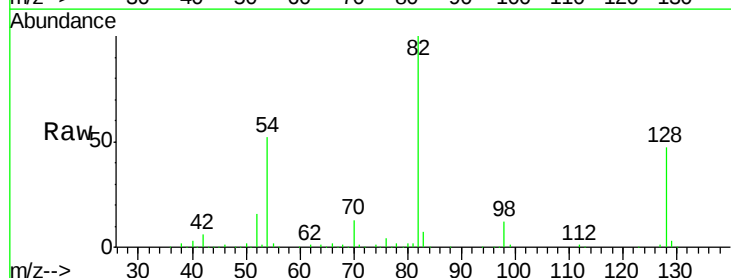

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1



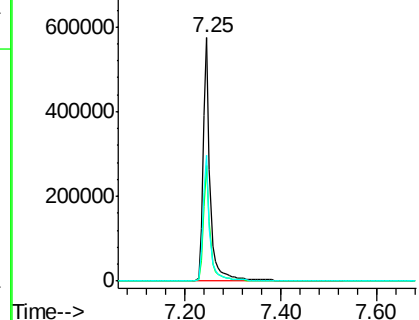



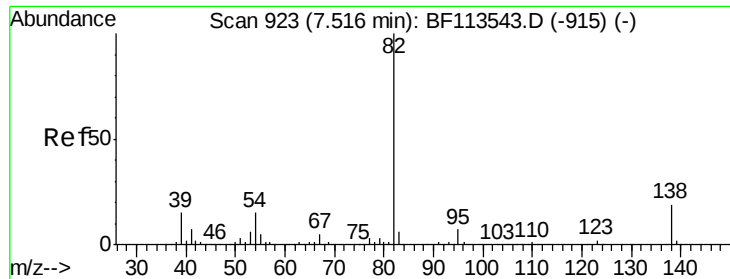

#25
Isophorone
Concen: 49.649 ng
RT: 7.25 min Scan# 877
Delta R.T. -0.27 min
Lab File: BF113679.D
Acq: 10 Apr 2019 2:04




Instrument :
BNA_F
ClientSampleId :

Tot Ion: 82 Resp: 601478
Ion Ratio Lower Upper
82 100
95 0.0 5.5 8.3#
138 0.0 15.2 22.8#

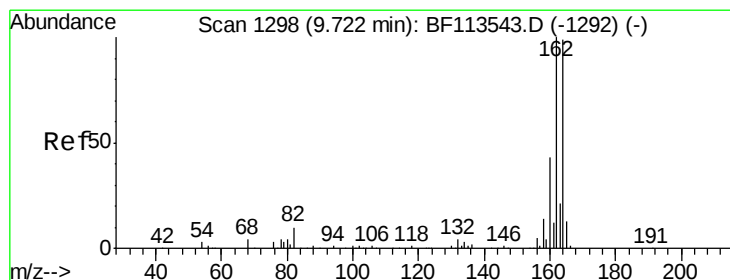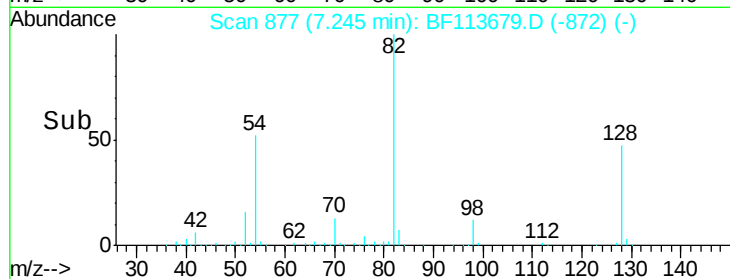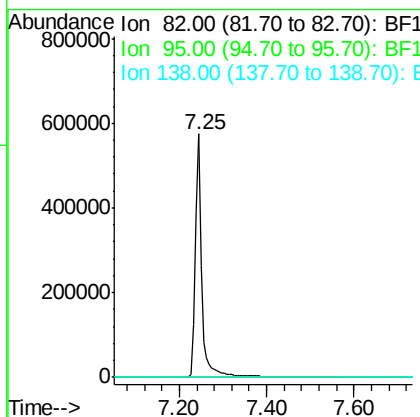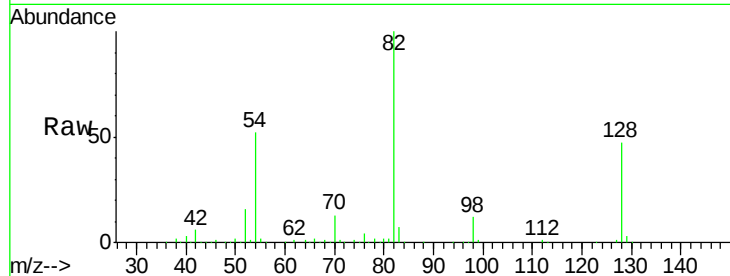

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.71 min Scan# 1296
Delta R.T. -0.01 min
Lab File: BF113679.D
Acq: 10 Apr 2019 2:04

Tgt Ion: 164 Resp: 169611
Ion Ratio Lower Upper
164 100
162 101.0 81.8 122.6
160 45.3 36.4 54.6

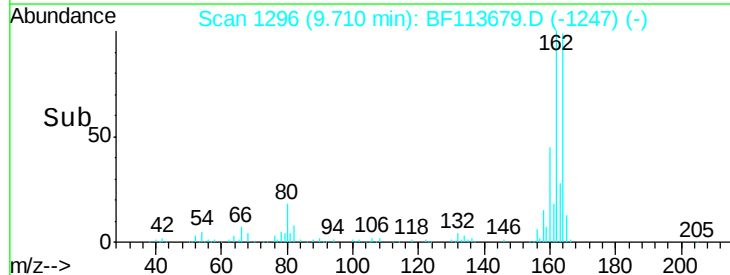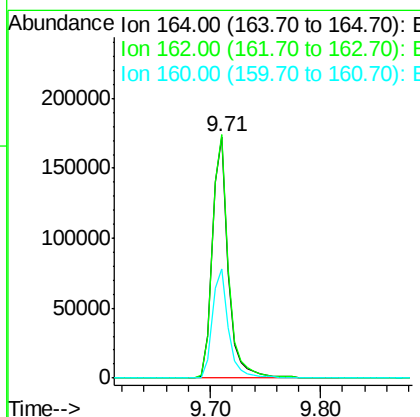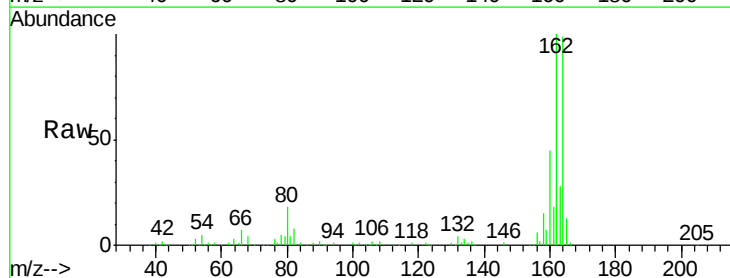







#42
 2,4,6-Tribromophenol
 Concen: 139.265 ng
 RT: 10.50 min Scan# 1430
 Delta R.T. -0.02 min
 Lab File: BF113679.D
 Acq: 10 Apr 2019 2:04

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:330 Resp: 283744
 Ion Ratio Lower Upper
 330 100
 332 96.0 77.8 116.6
 141 27.1 22.7 34.1

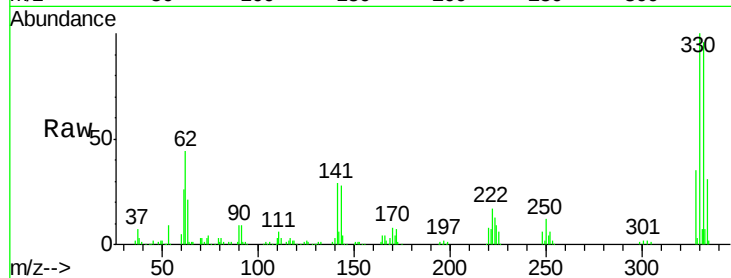


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

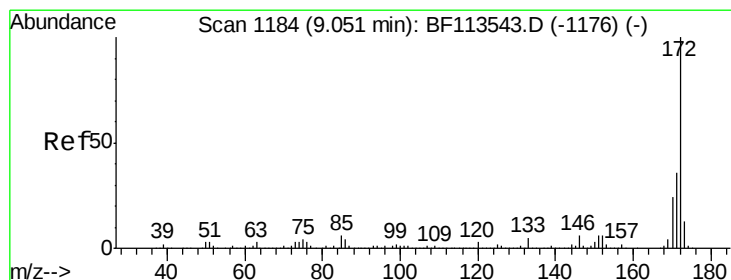
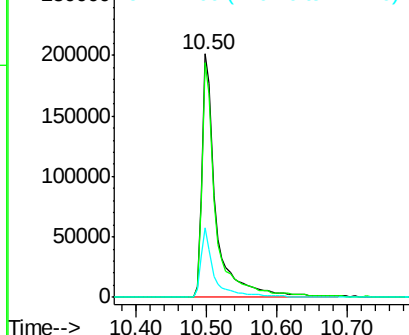



#45
 2-Fluorobiphenyl
 Concen: 105.109 ng
 RT: 9.03 min Scan# 1181
 Delta R.T. -0.02 min
 Lab File: BF113679.D
 Acq: 10 Apr 2019 2:04

Tgt Ion:172 Resp: 1107385
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.0 43.6
 170 24.4 19.5 29.3

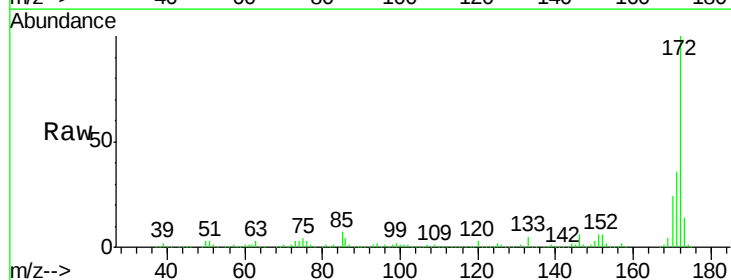

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

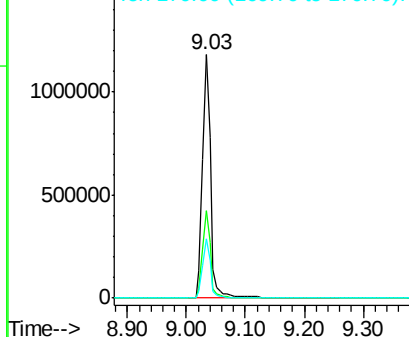

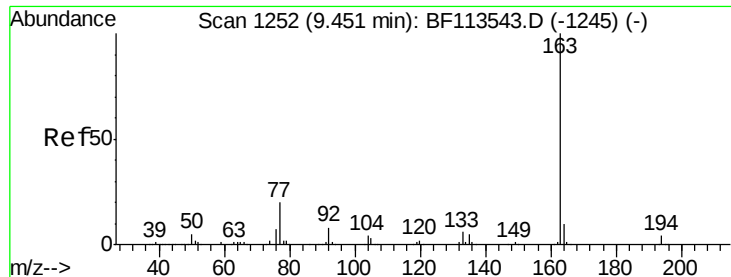

#50

Dimethylphthalate

Concen: 3.221 ng

RT: 9.71 min Scan# 1296

Delta R.T. 0.26 min

Lab File: BF113679.D

Acq: 10 Apr 2019 2:04

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 40266

Ion Ratio Lower Upper

163 100

194 0.0 3.0 4.6#




164 358.2 8.1 12.1#

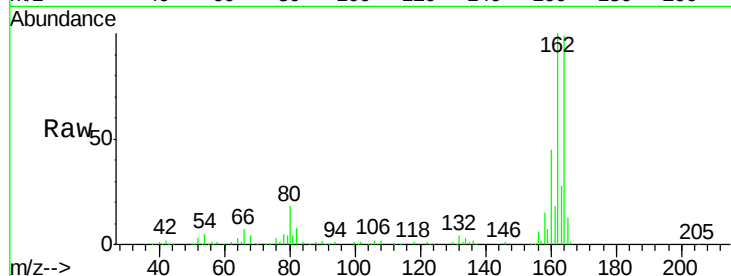

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

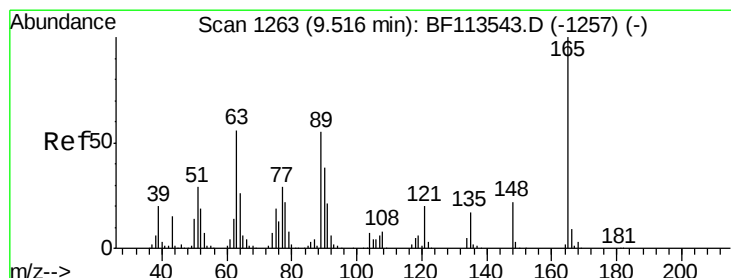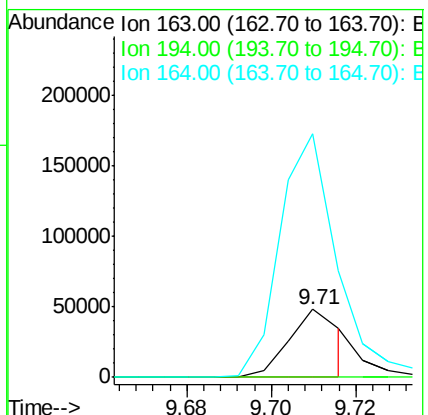

#51

2,6-Dinitrotoluene

Concen: 7.670 ng

RT: 9.71 min Scan# 1296

Delta R.T. 0.19 min

Lab File: BF113679.D

Acq: 10 Apr 2019 2:04


Tgt Ion:165 Resp: 21138

Ion Ratio Lower Upper

165 100

63 0.0 43.4 65.0#



89 0.0 43.1 64.7#

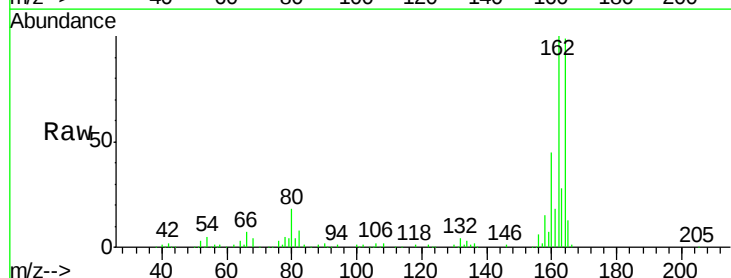


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

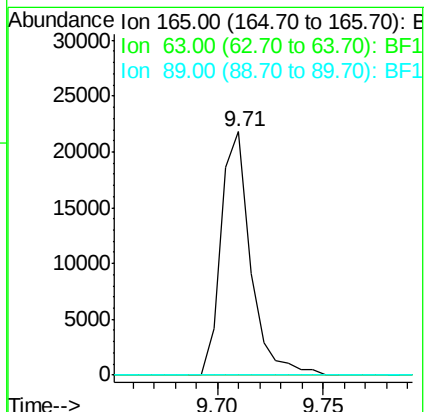

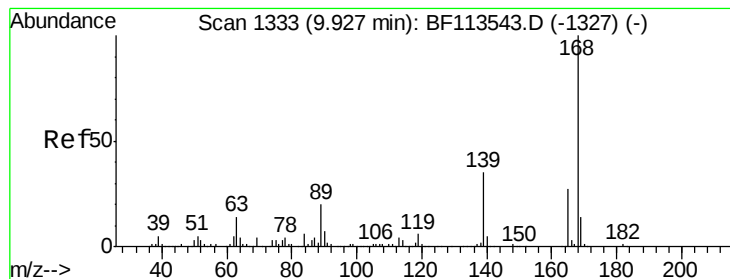

#57

2,4-Dinitrotoluene

Concen: 6.342 ng

RT: 9.71 min Scan# 1296

Delta R.T. -0.22 min

Lab File: BF113679.D

Acq: 10 Apr 2019 2:04

Instrument :

BNA_F

ClientSampleId :

Tot Ion:165 Resp: 21138


Ion Ratio Lower Upper

165 100

63 0.0 37.5 56.3#

89 0.0 57.4 86.2#

182 0.0 2.0 3.0#

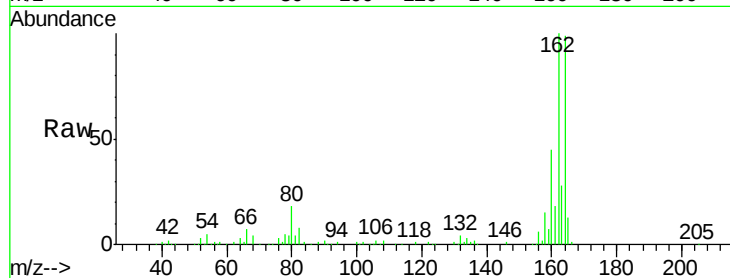


Abundance Ion 165.00 (164.70 to 165.70): E



Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

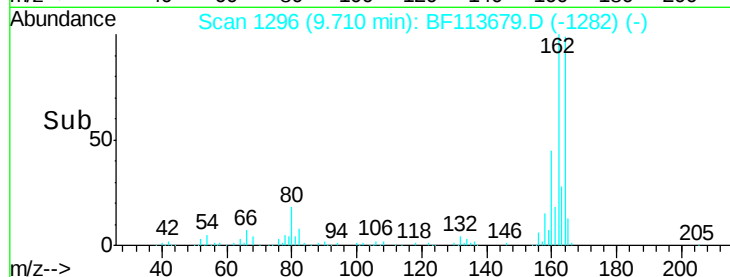

Time-->

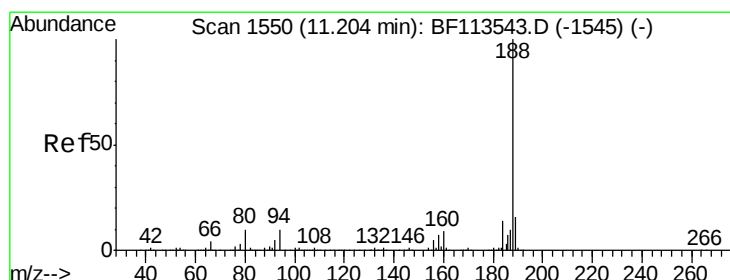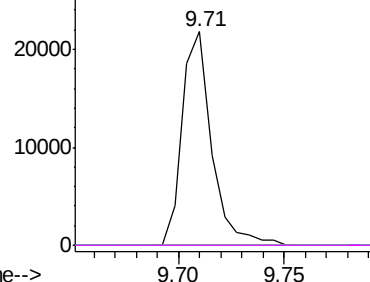

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.19 min Scan# 1548

Delta R.T. -0.01 min

Lab File: BF113679.D

Acq: 10 Apr 2019 2:04


Tgt Ion:188 Resp: 311316

Ion Ratio Lower Upper

188 100

94 8.9 7.0 10.6


80 8.7 7.7 11.5

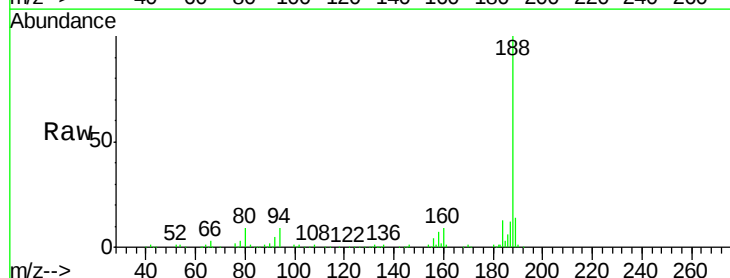


Abundance Ion 188.00 (187.70 to 188.70): E


Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

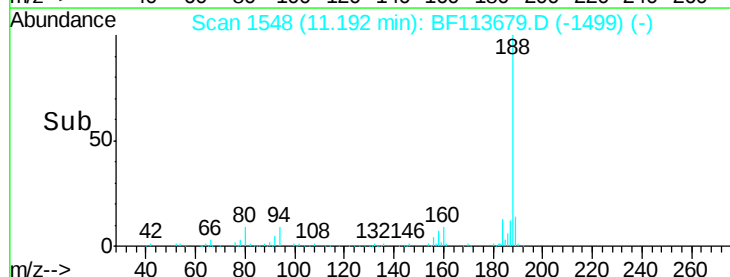

Time-->

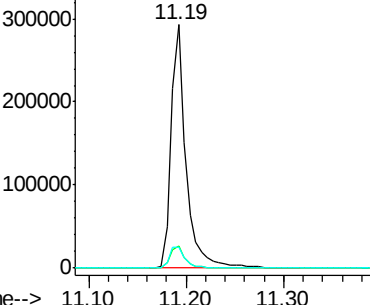


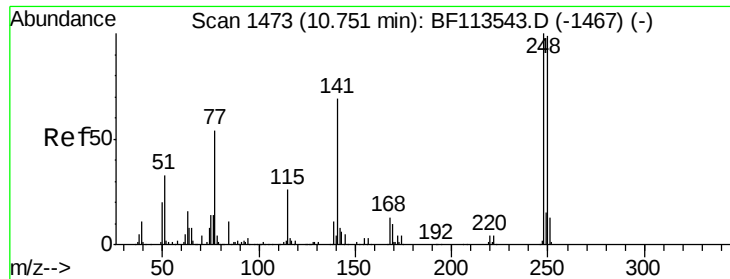




#67
4-Bromophenyl-phenylether
Concen: 4.159 ng
RT: 10.50 min Scan# 1430
Delta R.T. -0.25 min
Lab File: BF113679.D
Acq: 10 Apr 2019 2:04

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 14522
Ion Ratio Lower Upper
248 100
250 198.4 78.3 117.5#
141 484.0 56.2 84.4#

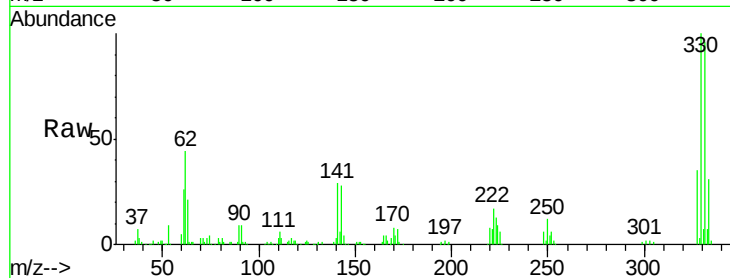


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

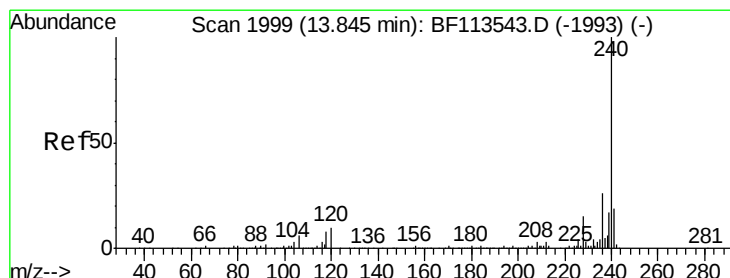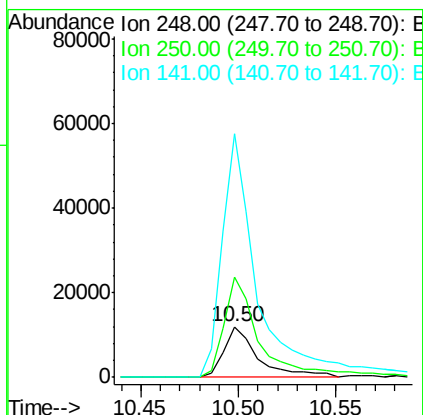
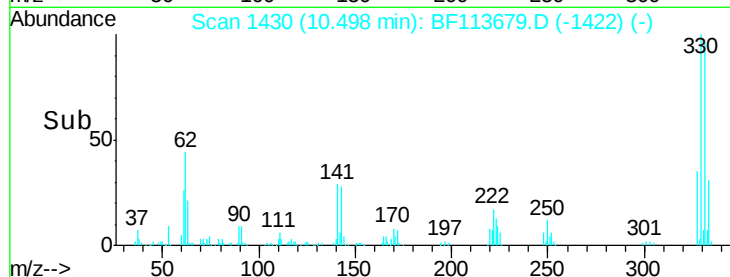



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.83 min Scan# 1996
Delta R.T. -0.02 min
Lab File: BF113679.D
Acq: 10 Apr 2019 2:04

Tgt Ion:240 Resp: 259043
Ion Ratio Lower Upper
240 100
120 9.8 8.8 13.2
236 25.2 20.9 31.3

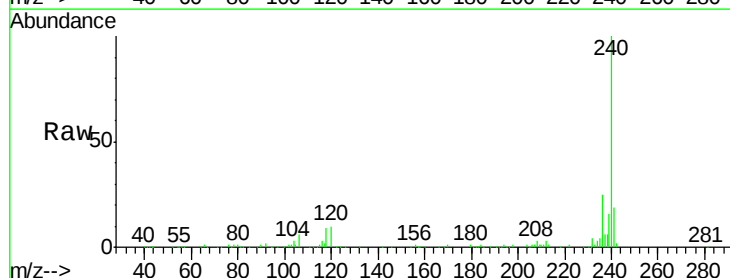

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

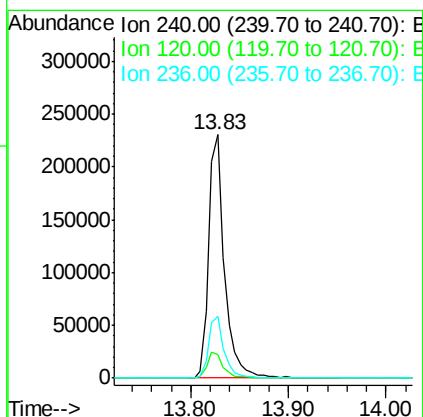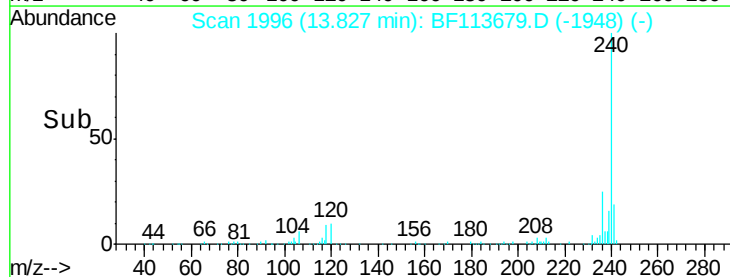







#79
 Terphenyl-d14
 Concen: 83.777 ng
 RT: 12.77 min Scan# 1816
 Delta R.T. -0.02 min
 Lab File: BF113679.D
 Acq: 10 Apr 2019 2:04

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:244 Resp: 1065900

Ion	Ratio	Lower	Upper
244	100		
212	6.6	5.5	8.3
122	11.5	8.6	13.0

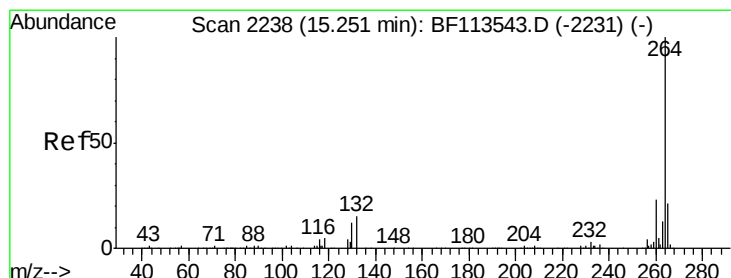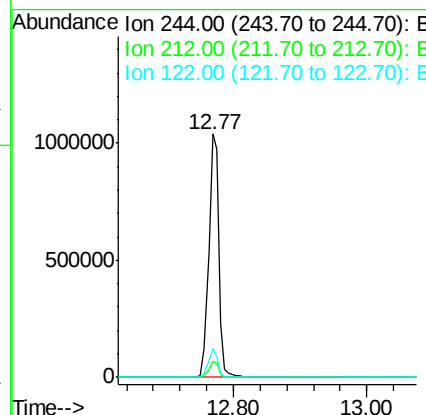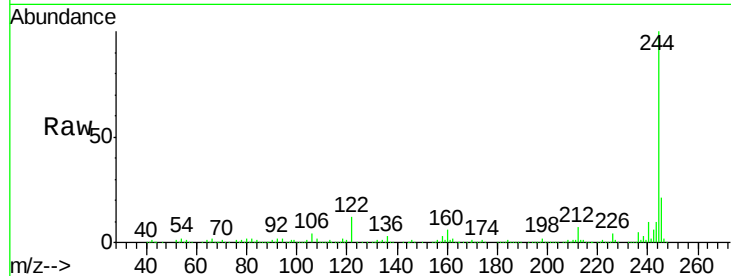

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.23 min Scan# 2235
 Delta R.T. -0.02 min
 Lab File: BF113679.D
 Acq: 10 Apr 2019 2:04

Tgt Ion:264 Resp: 257996

Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.1	28.7
265	21.2	17.1	25.7

