
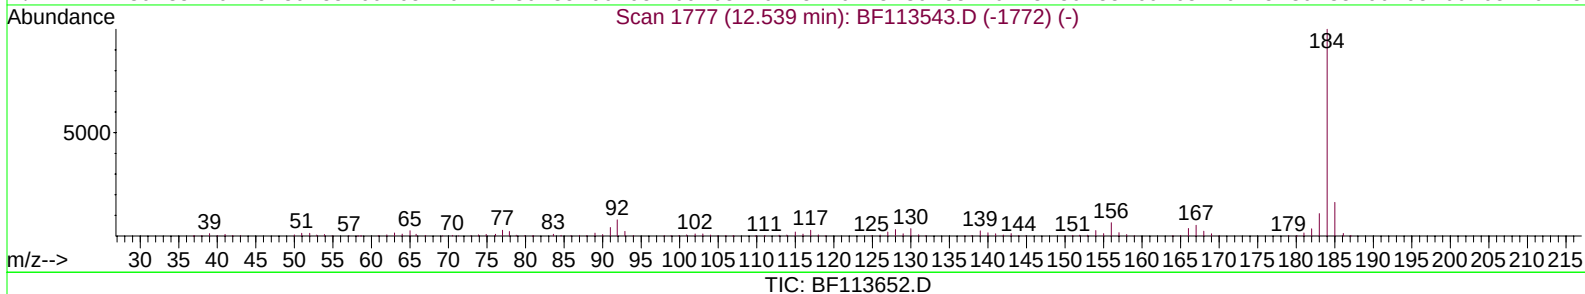
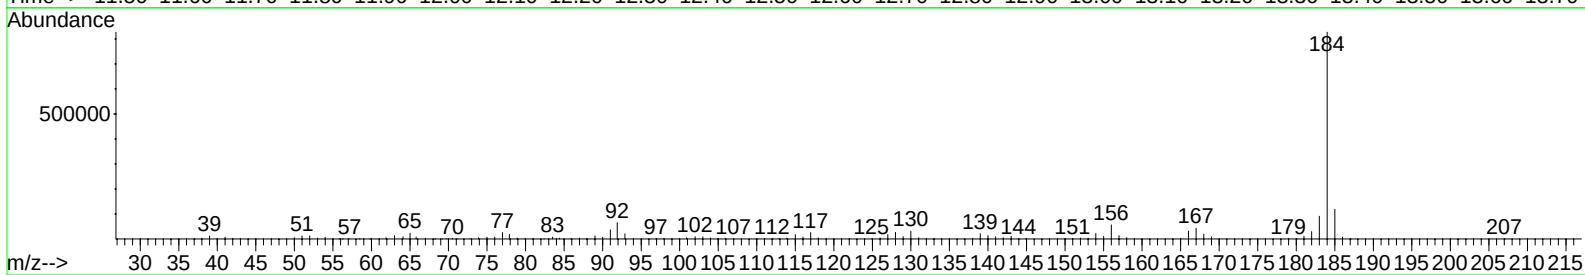


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040919\  
Data File   : BF113652.D  
Acq On      : 9 Apr 2019    9:51  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Apr 09 18:56:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

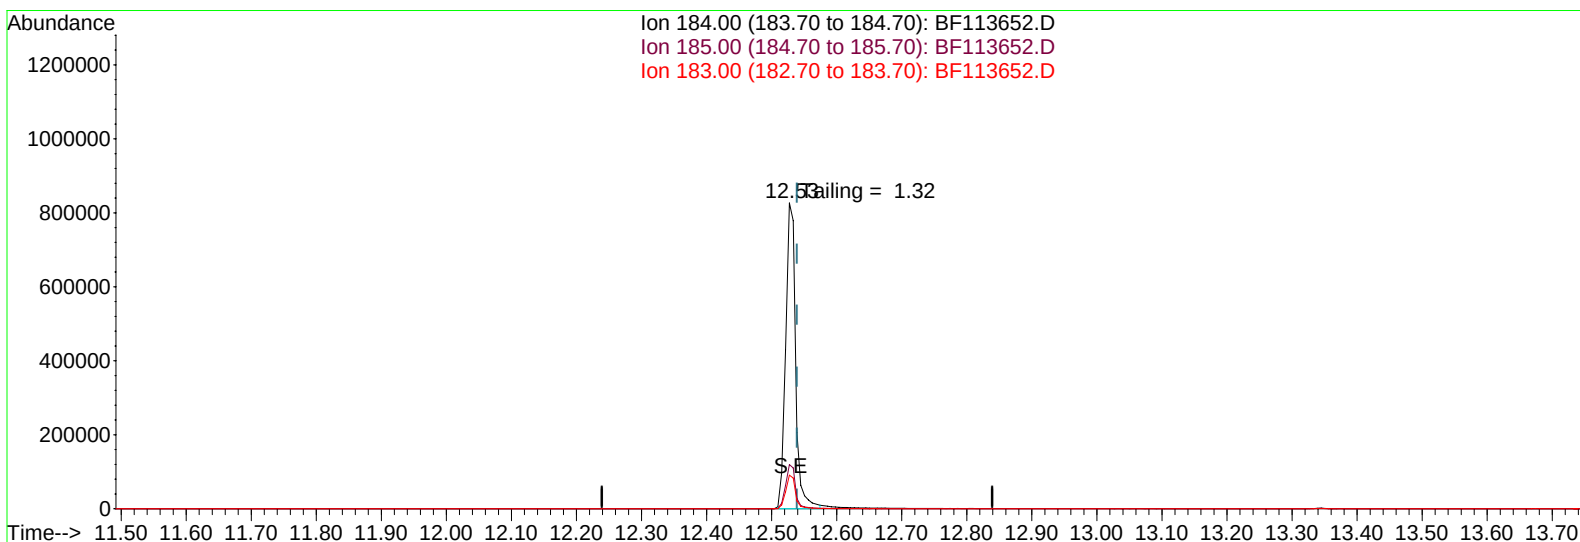

(77) Benzidine




12.527min (-0.012) 0.00ng

response 908753

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.44
183.00	11.20	10.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040919\
Data File : BF113652.D
Acq On : 9 Apr 2019 9:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 18:56:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

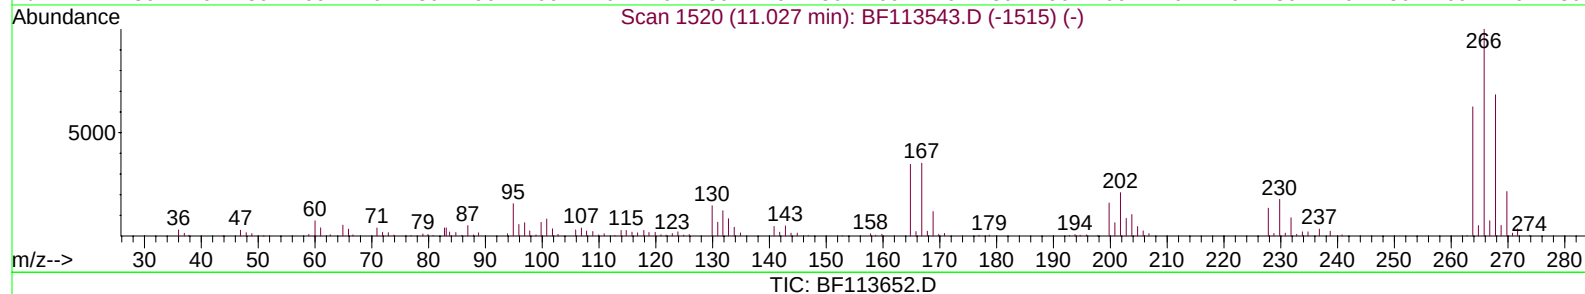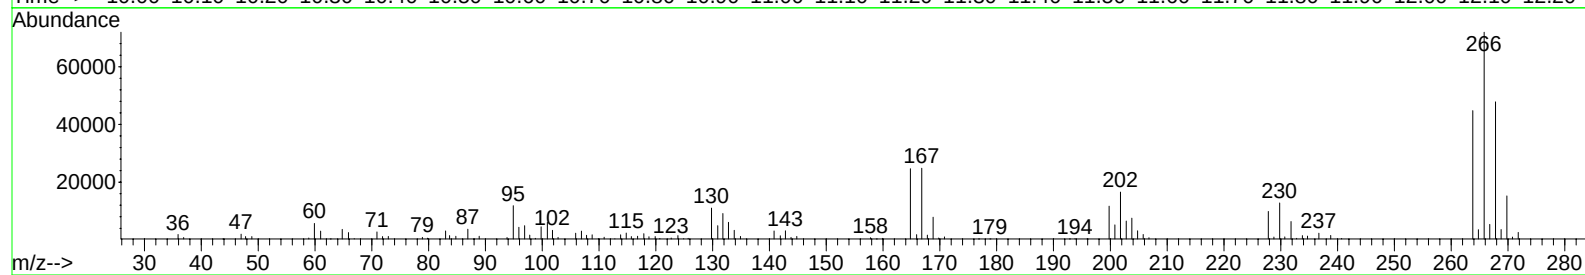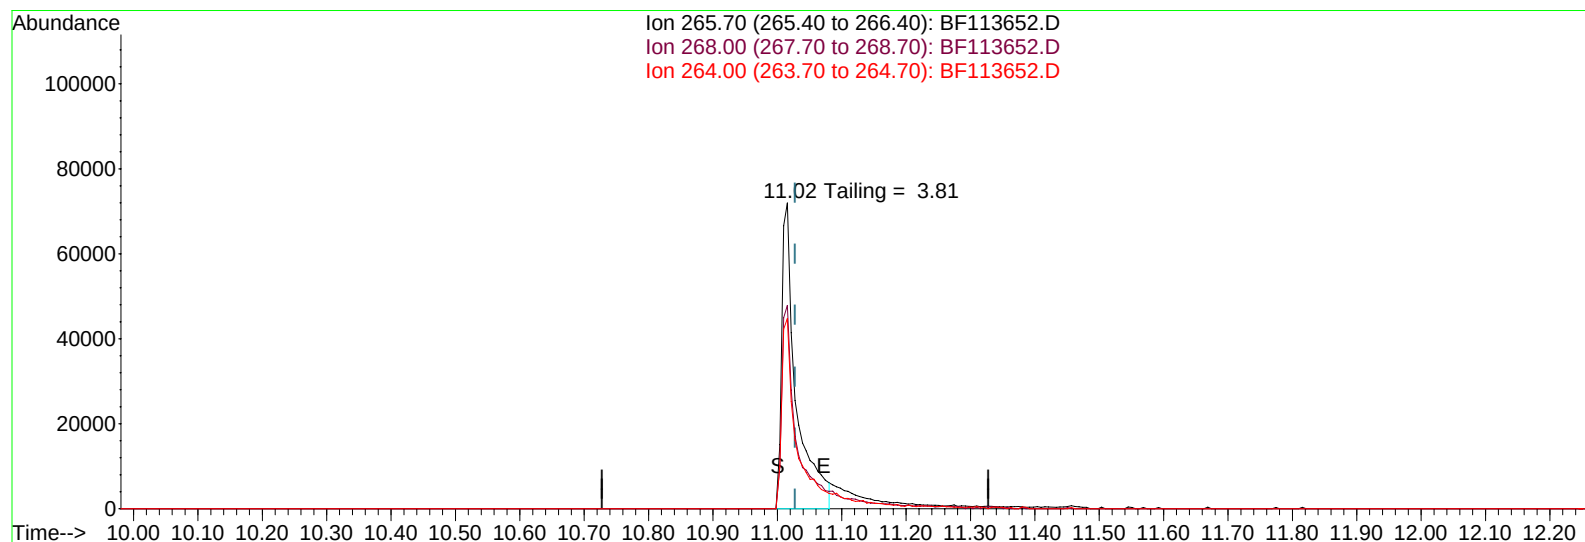

(70) Pentachlorophenol (C)

11.016min (-0.012) 34117.23ng

response 135940

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	66.51
264.00	61.50	62.23
0.00	0.00	0.00