

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040919\
 Data File : BF113662.D
 Acq On : 9 Apr 2019 15:37
 Operator : JU/SJ
 Sample : K2316-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20190176-AMND-COMP-CS-3

Quant Time: Apr 10 05:59:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	106214	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	402832	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	197953	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	403054	20.00	ng	-0.01
76) Chrysene-d12	13.83	240	306157	20.00	ng	-0.02
87) Perylene-d12	15.23	264	291342	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	556194	89.30	ng	0.00
7) Phenol-d6	6.33	99	976963	127.26	ng	0.00
23) Nitrobenzene-d5	7.25	82	569527	82.81	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	211383	88.89	ng	-0.02
45) 2-Fluorobiphenyl	9.03	172	1022020	83.12	ng	-0.02
79) Terphenyl-d14	12.77	244	1123280	74.70	ng	-0.02
Target Compounds						
50) Dimethylphthalate	9.43	163	152821	10.473	ng	99
84) Bis(2-ethylhexyl)phthalate	13.80	149	139784	12.192	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040919\
Data File : BF113662.D
Acq On : 9 Apr 2019 15:37
Operator : JU/SJ
Sample : K2316-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20190176-AMND-COMP-CS-3

Quant Time: Apr 10 05:59:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

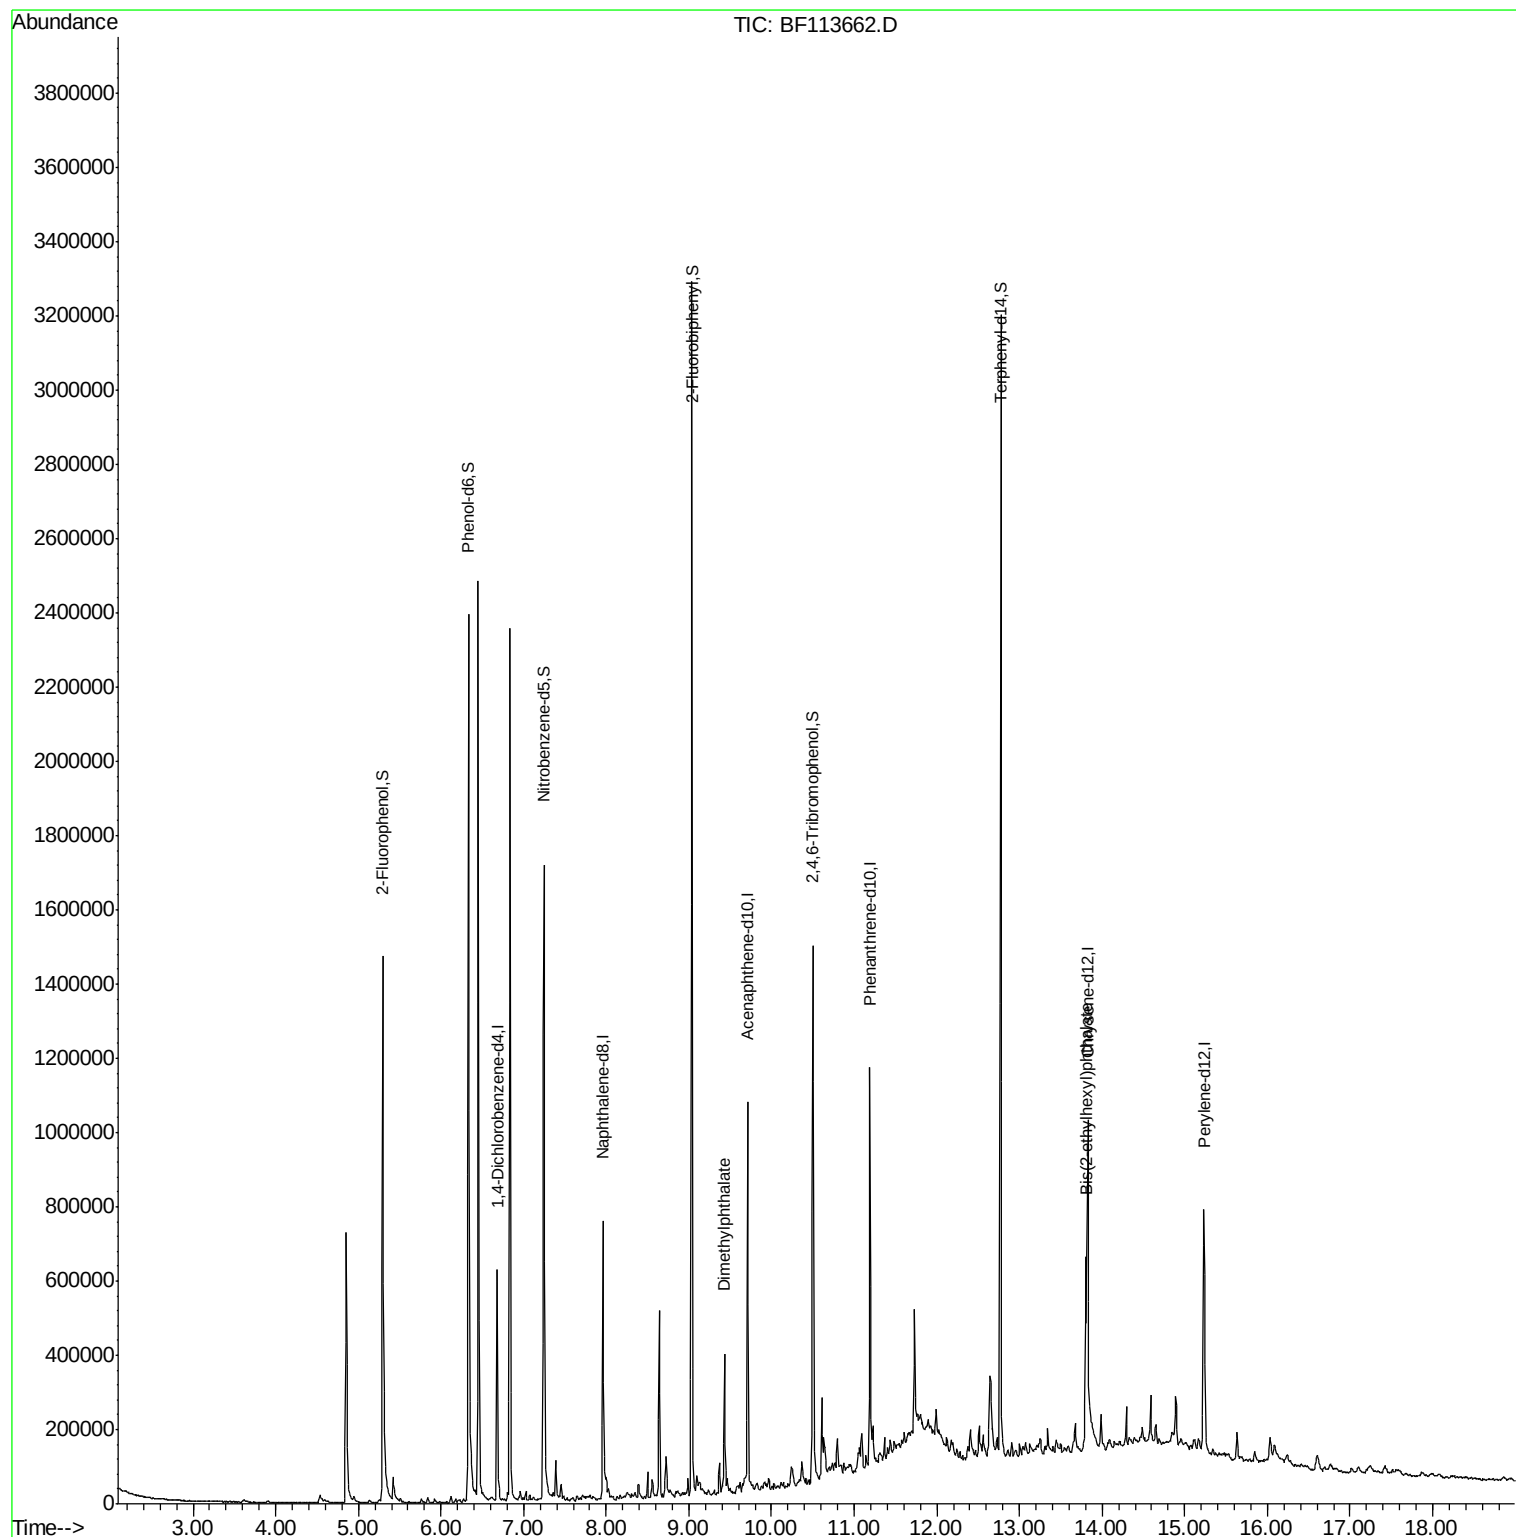

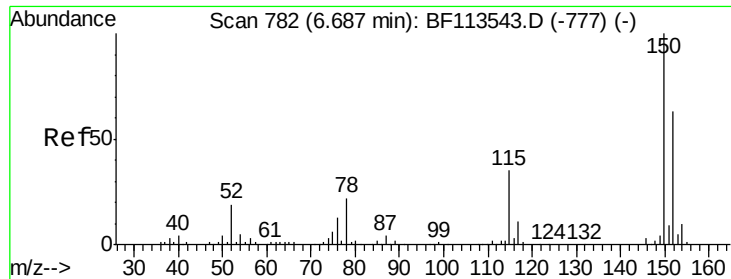


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.68 min Scan# 781
Delta R.T. -0.01 min
Lab File: BF113662.D
Acq: 9 Apr 2019 15:37

Instrument :
BNA_F
ClientSampleId :
20190176-AMND-COMP-CS-3

Tgt Ion:152 Resp: 106214
Ion Ratio Lower Upper
152 100
150 153.2 124.7 187.1
115 54.4 46.0 69.0

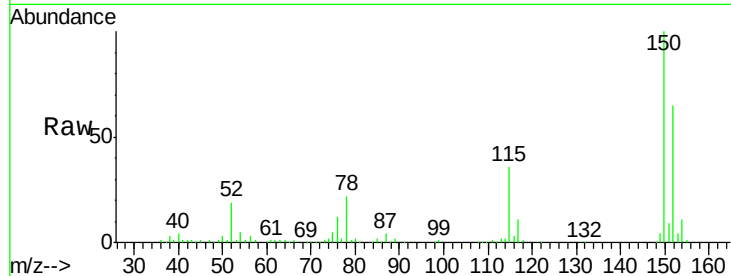


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

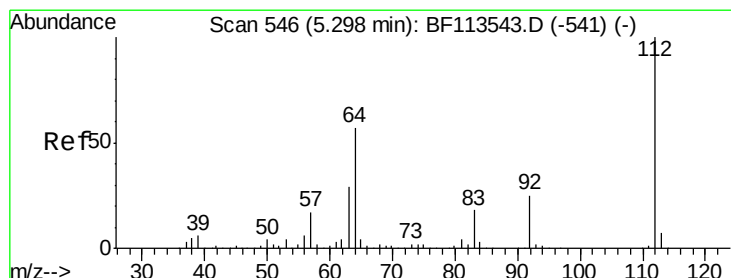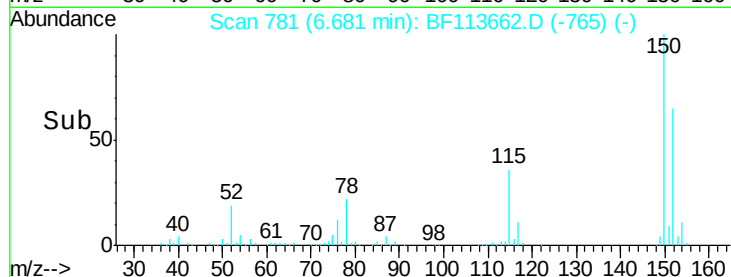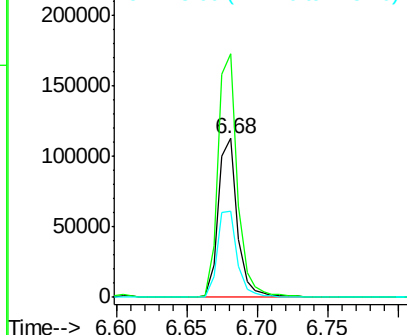



#5


2-Fluorophenol
Concen: 89.295 ng
RT: 5.29 min Scan# 545
Delta R.T. -0.01 min
Lab File: BF113662.D
Acq: 9 Apr 2019 15:37

Tgt Ion:112 Resp: 556194
Ion Ratio Lower Upper
112 100
64 60.6 49.2 73.8
63 30.8 24.9 37.3

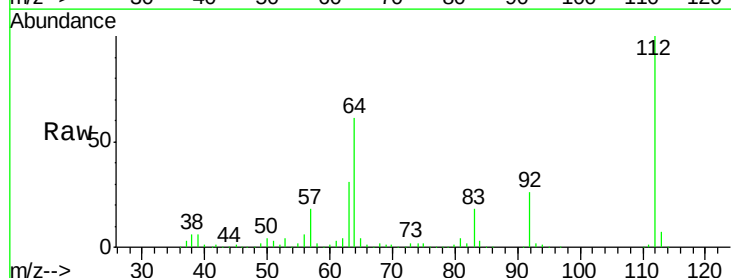

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

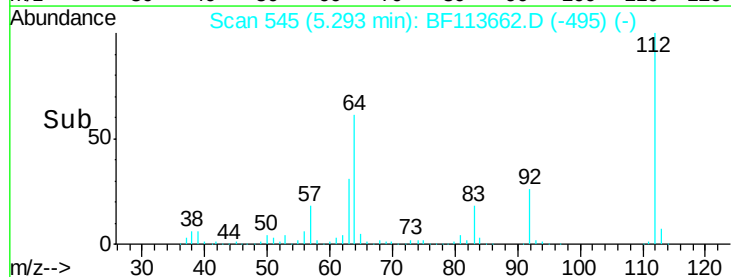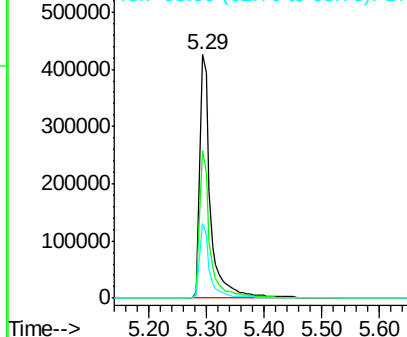

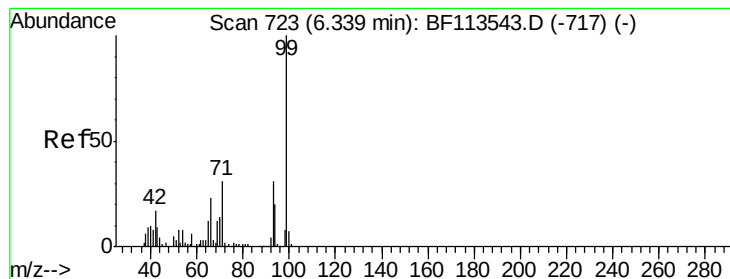

#7

Phenol-d6

Concen: 127.260 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37

Instrument :

BNA_F

ClientSampleId :

20190176-AMND-COMP-CS-3





Tgt Ion: 99 Resp: 976963

Ion Ratio Lower Upper

99 100

42 18.4 14.8 22.2

71 32.0 24.9 37.3

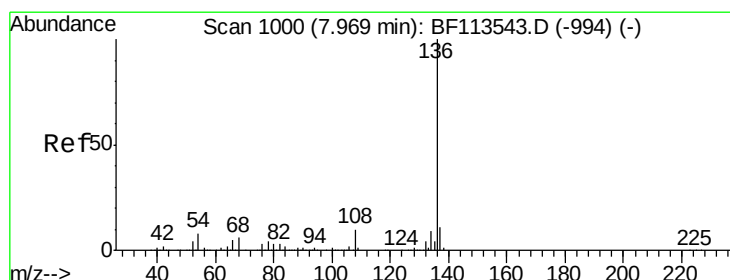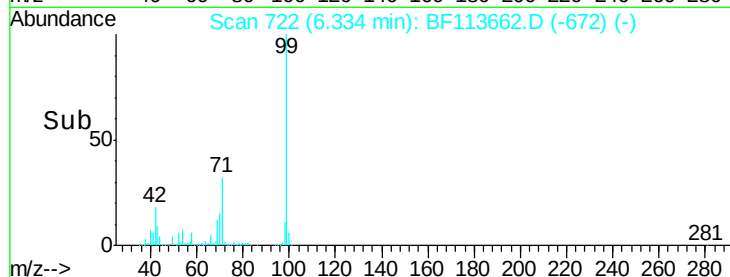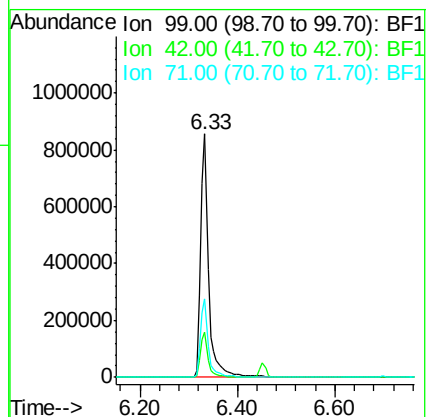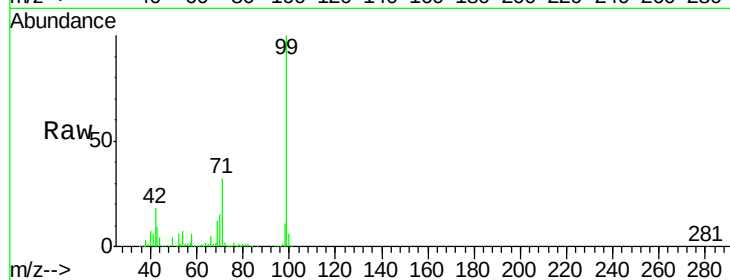

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37

Tgt Ion: 136 Resp: 402832




Ion Ratio Lower Upper


136 100

137 10.7 8.9 13.3

54 7.6 7.0 10.6

68 5.7 4.8 7.2

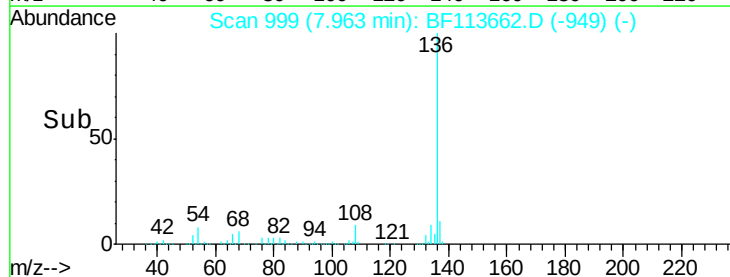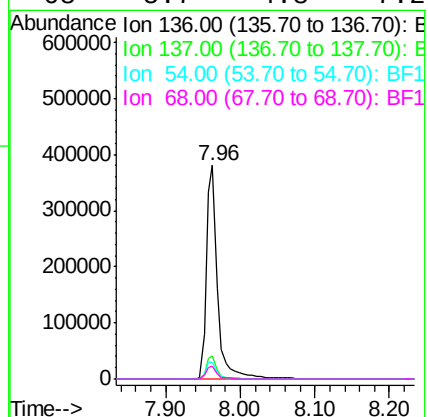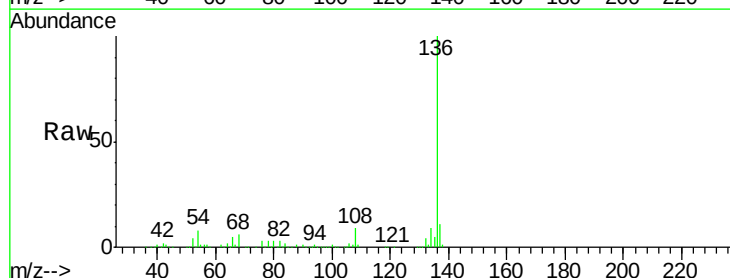

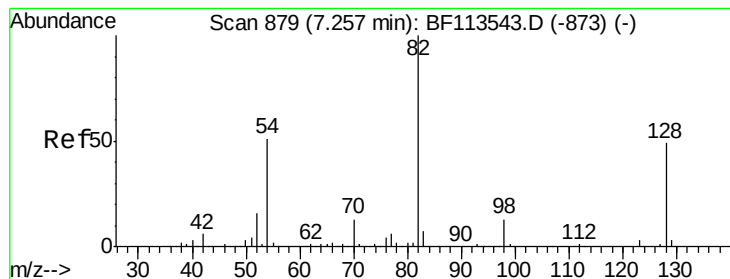

#23

Nitrobenzene-d5

Concen: 82.814 ng

RT: 7.25 min Scan# 877

Delta R.T. -0.01 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37





Instrument :

BNA_F

ClientSampleId :

20190176-AMND-COMP-CS-3

Tgt Ion:	82	Resp:	569527
Ion	Ratio	Lower	Upper
82	100		
128	47.9	36.5	54.7
54	50.9	42.2	63.2

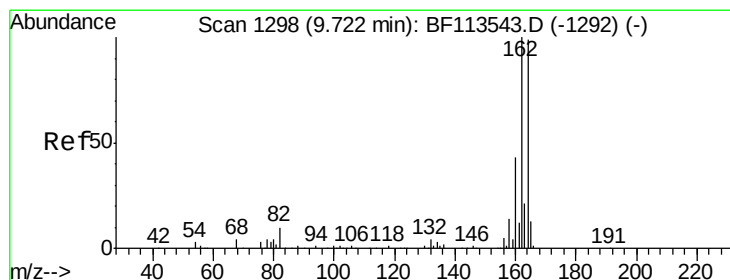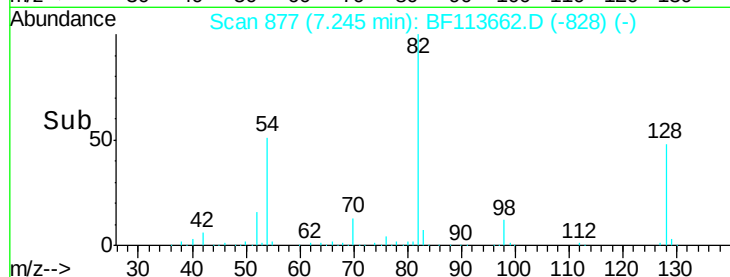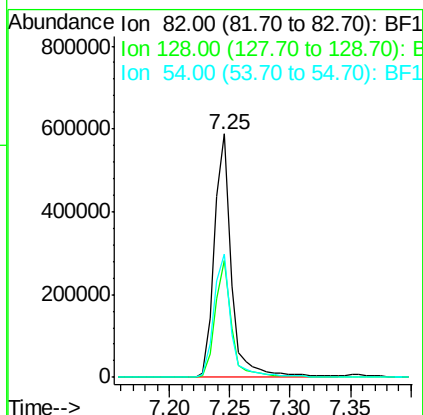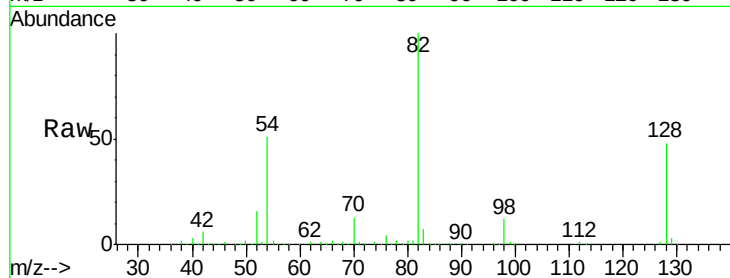

#39

Acenaphthene-d10

Concen: 20.000 ng




RT: 9.71 min Scan# 1296


Delta R.T. -0.01 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37

Tgt Ion:	164	Resp:	197953
Ion	Ratio	Lower	Upper
164	100		
162	99.5	81.8	122.6
160	44.3	36.4	54.6

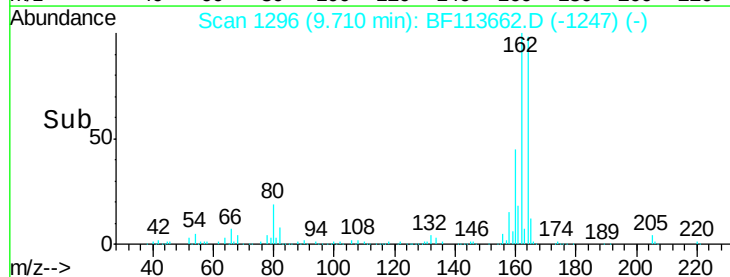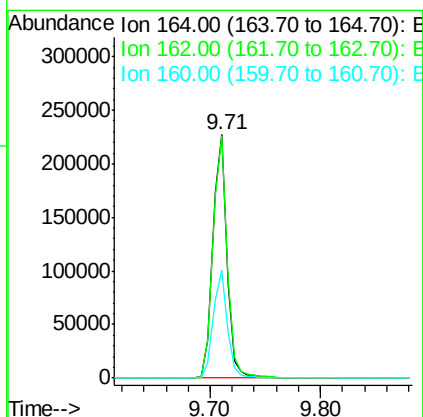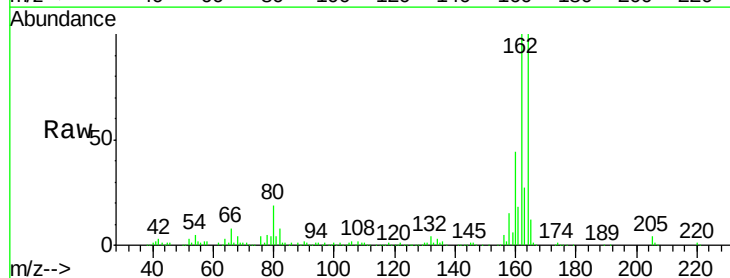


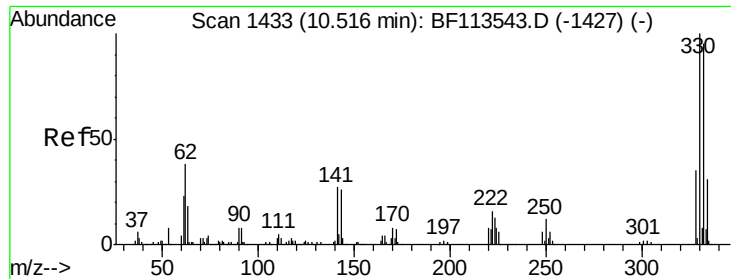




#42
 2,4,6-Tribromophenol
 Concen: 88.895 ng
 RT: 10.50 min Scan# 1430
 Delta R.T. -0.02 min
 Lab File: BF113662.D
 Acq: 9 Apr 2019 15:37

Instrument :
 BNA_F
 ClientSampleId :
 20190176-AMND-COMP-CS-3

Tgt Ion:330 Resp: 211383
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.8 116.6
 141 27.9 22.7 34.1

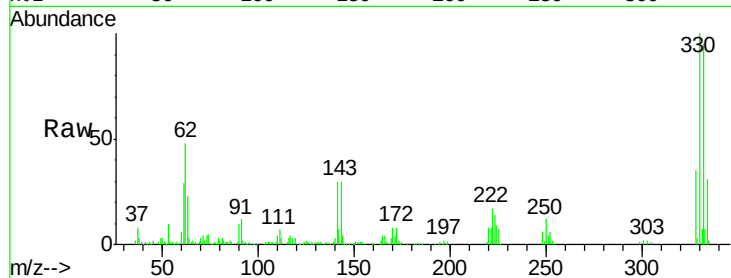


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

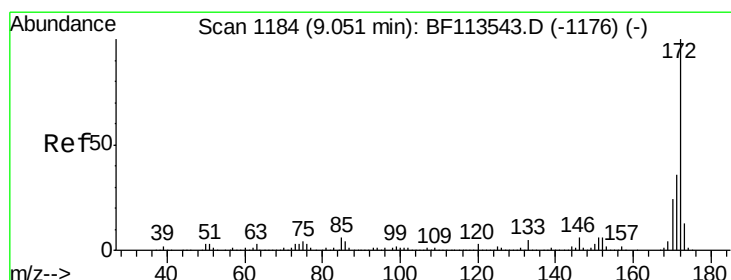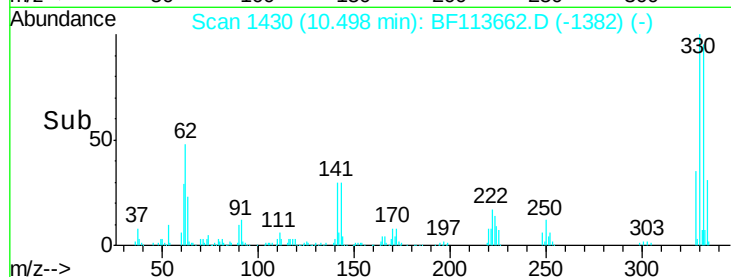
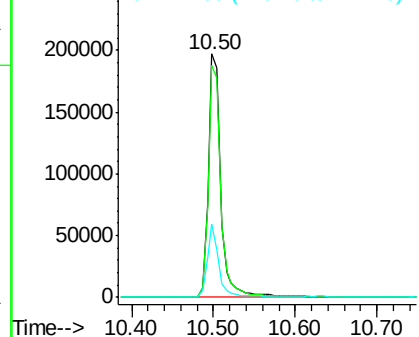



#45
 2-Fluorobiphenyl
 Concen: 83.118 ng
 RT: 9.03 min Scan# 1181
 Delta R.T. -0.02 min
 Lab File: BF113662.D
 Acq: 9 Apr 2019 15:37

Tgt Ion:172 Resp: 1022020
 Ion Ratio Lower Upper
 172 100
 171 35.3 29.0 43.6
 170 24.1 19.5 29.3

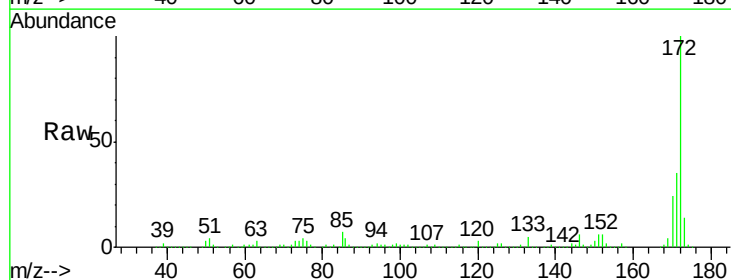

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

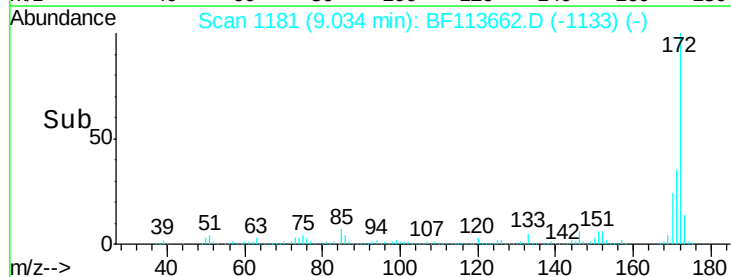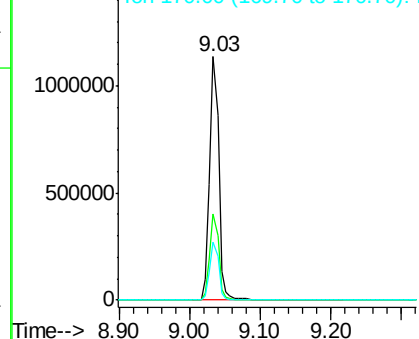

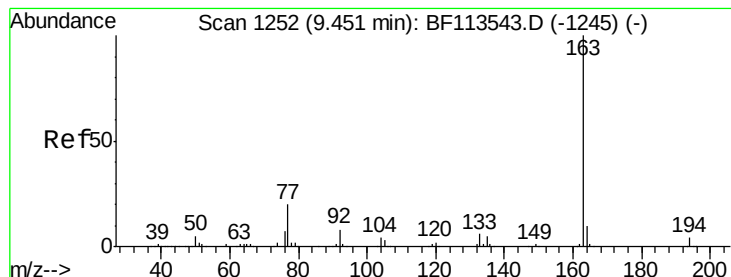

#50

Dimethylphthalate

Concen: 10.473 ng

RT: 9.43 min Scan# 1248

Delta R.T. -0.02 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37

Instrument :

BNA_F

ClientSampleId :

20190176-AMND-COMP-CS-3


Tgt Ion:163 Resp: 152821

Ion Ratio Lower Upper

163 100

194 3.8 3.0 4.6

164 10.6 8.1 12.1

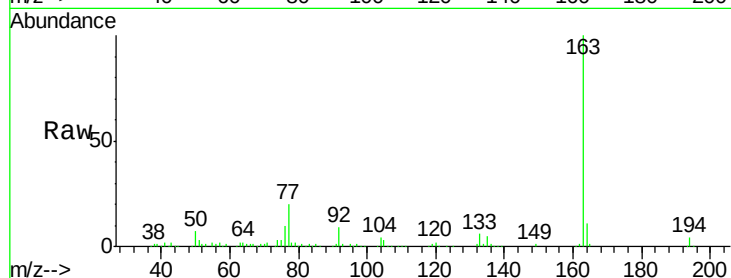

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

9.43



150000

100000

50000

0

Time-->

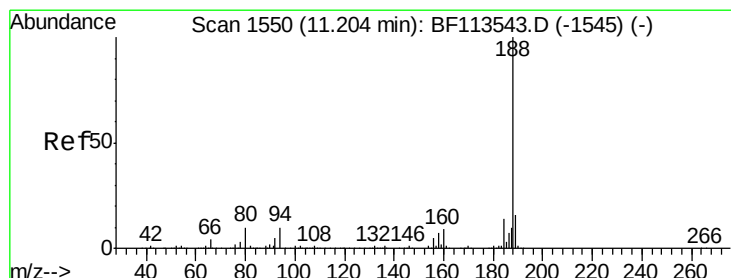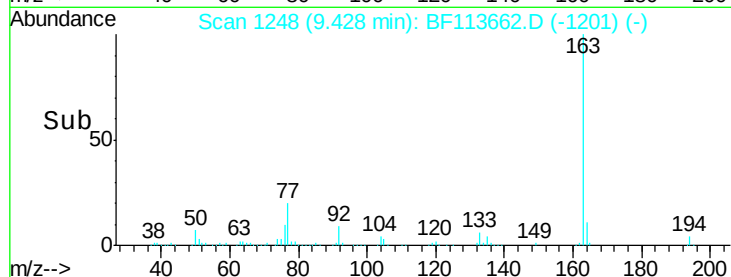

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.19 min Scan# 1548

Delta R.T. -0.01 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37


Tgt Ion:188 Resp: 403054

Ion Ratio Lower Upper

188 100

94 8.7 7.0 10.6

80 8.8 7.7 11.5

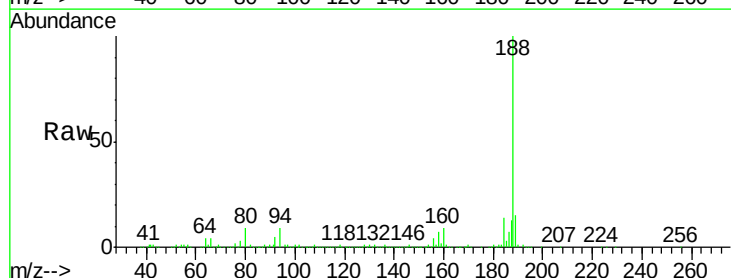

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

11.19

600000

500000

400000


300000


200000

100000

0

Time-->

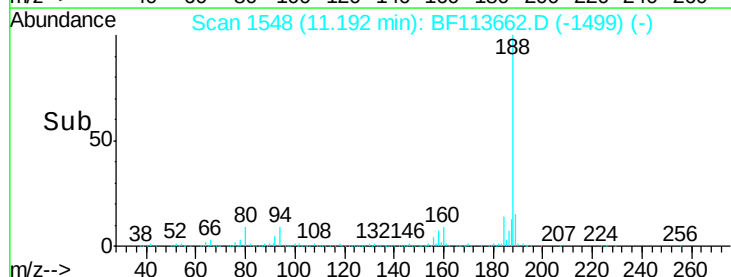

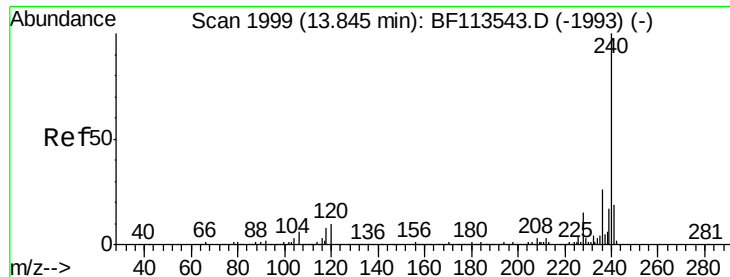

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1996

Delta R.T. -0.02 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37





Instrument :

BNA_F

ClientSampleId :

20190176-AMND-COMP-CS-3

Tgt Ion:	240	Resp:	306157
Ion	Ratio	Lower	Upper
240	100		
120	10.1	8.8	13.2
236	25.2	20.9	31.3

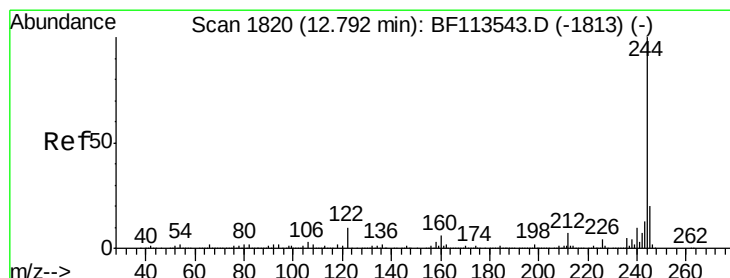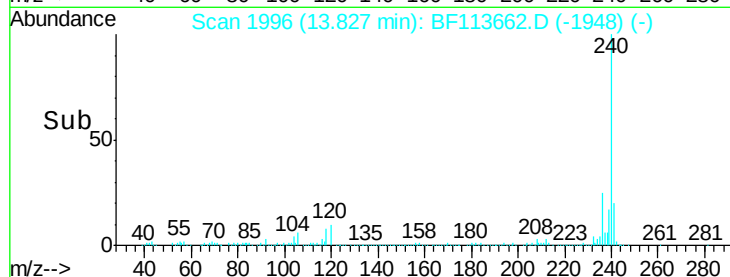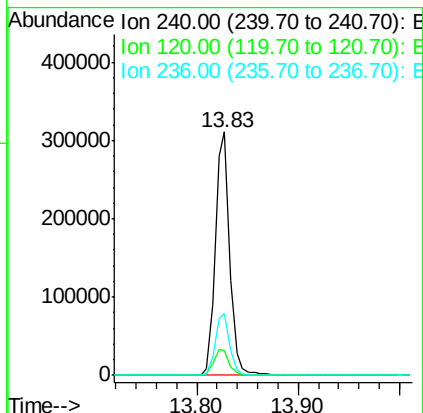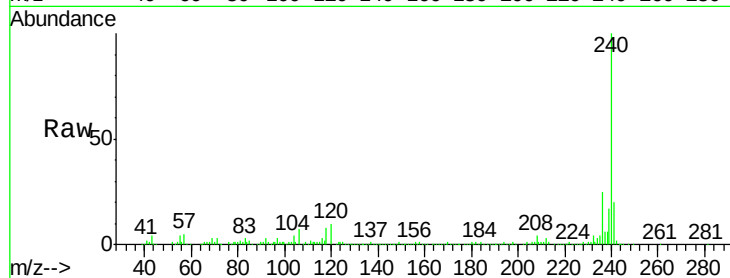

#79

Terphenyl-d14

Concen: 74.701 ng




RT: 12.77 min Scan# 1817


Delta R.T. -0.02 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37

Tgt Ion:	244	Resp:	1123280
Ion	Ratio	Lower	Upper
244	100		
212	6.6	5.5	8.3
122	10.0	8.6	13.0

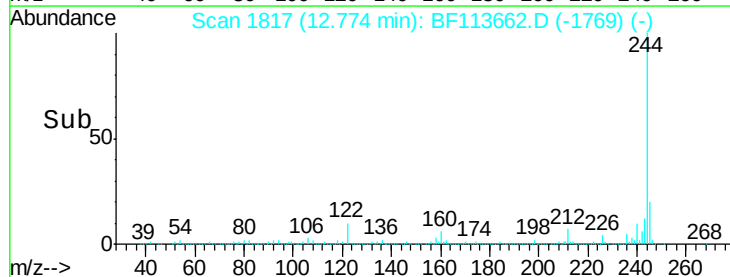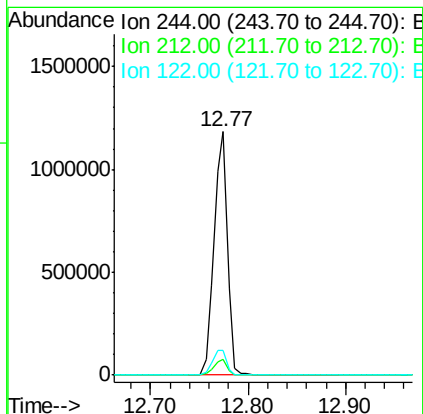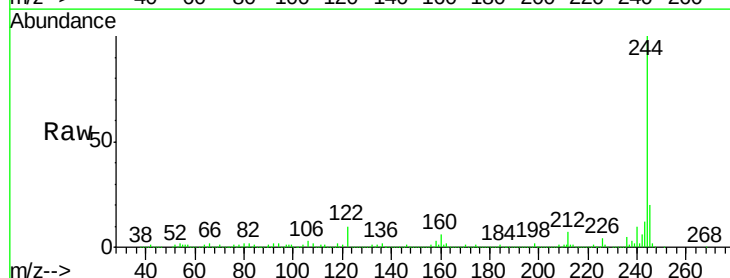

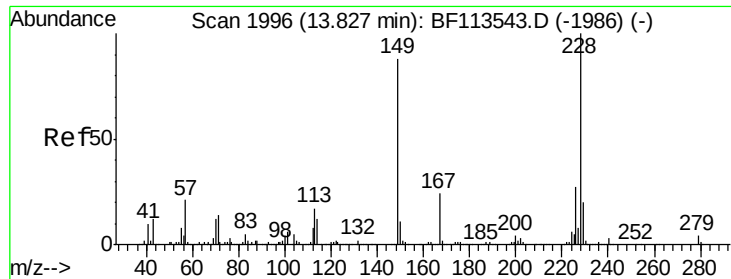

#84

Bis(2-ethylhexyl)phthalate

Concen: 12.192 ng

RT: 13.80 min Scan# 1992

Delta R.T. -0.02 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37

Instrument :

BNA_F

ClientSampleId :

20190176-AMND-COMP-CS-3


Tgt Ion:149 Resp: 139784

Ion Ratio Lower Upper

149 100

167 26.7 21.8 32.8




279 4.0 2.9 4.3

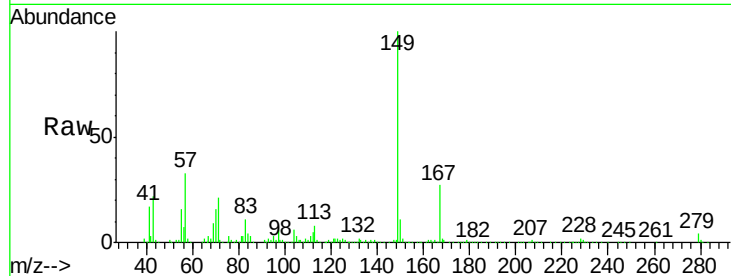

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

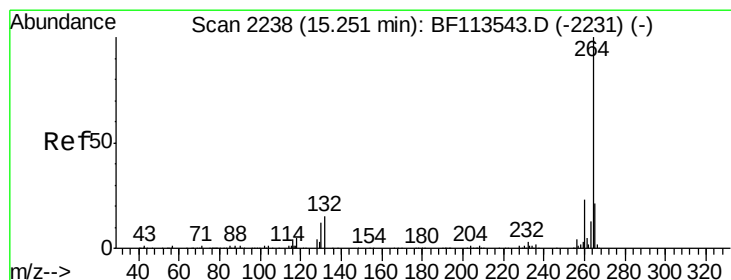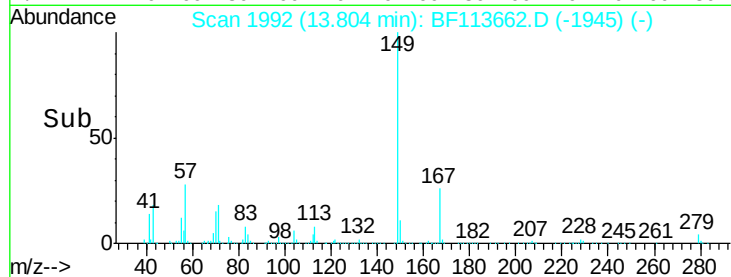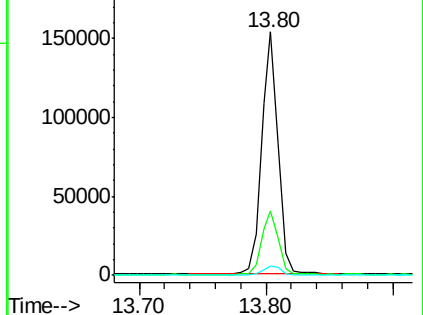

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.23 min Scan# 2235

Delta R.T. -0.02 min

Lab File: BF113662.D

Acq: 9 Apr 2019 15:37


Tgt Ion:264 Resp: 291342

Ion Ratio Lower Upper

264 100

260 23.3 19.1 28.7

265 21.7 17.1 25.7

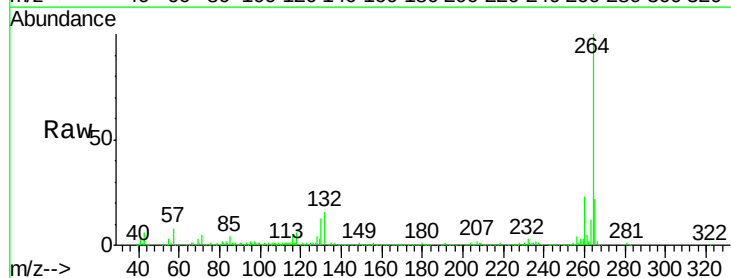

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

