


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040919\
 Data File : BF113652.D
 Acq On : 9 Apr 2019 9:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

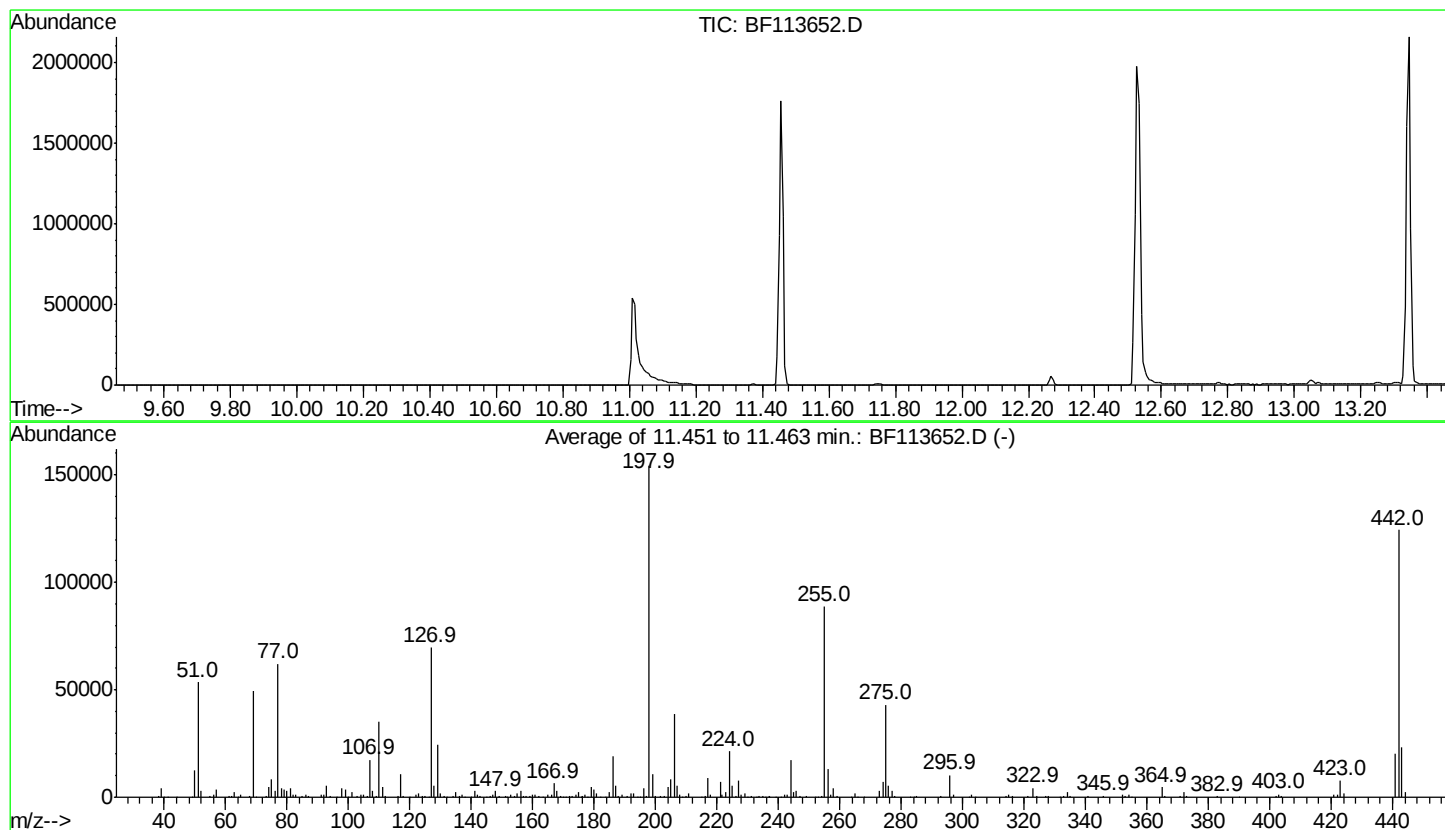

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	53373	PASS
68	69	0.00	2	1.8	878	PASS
69	198	0.00	100	32.2	49698	PASS
70	69	0.00	2	0.3	139	PASS
127	198	10	80	45.1	69581	PASS
197	198	0.00	2	0.4	640	PASS
198	198	100	100	100.0	154309	PASS
199	198	5	9	6.8	10518	PASS
275	198	10	60	27.8	42957	PASS
365	198	1	100	3.1	4744	PASS
441	198	0.01	100	13.2	20306	PASS
442	198	50	100	80.6	124381	PASS
443	442	15	24	18.9	23460	PASS