


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040919\
 Data File : BF113677.D
 Acq On : 10 Apr 2019 00:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

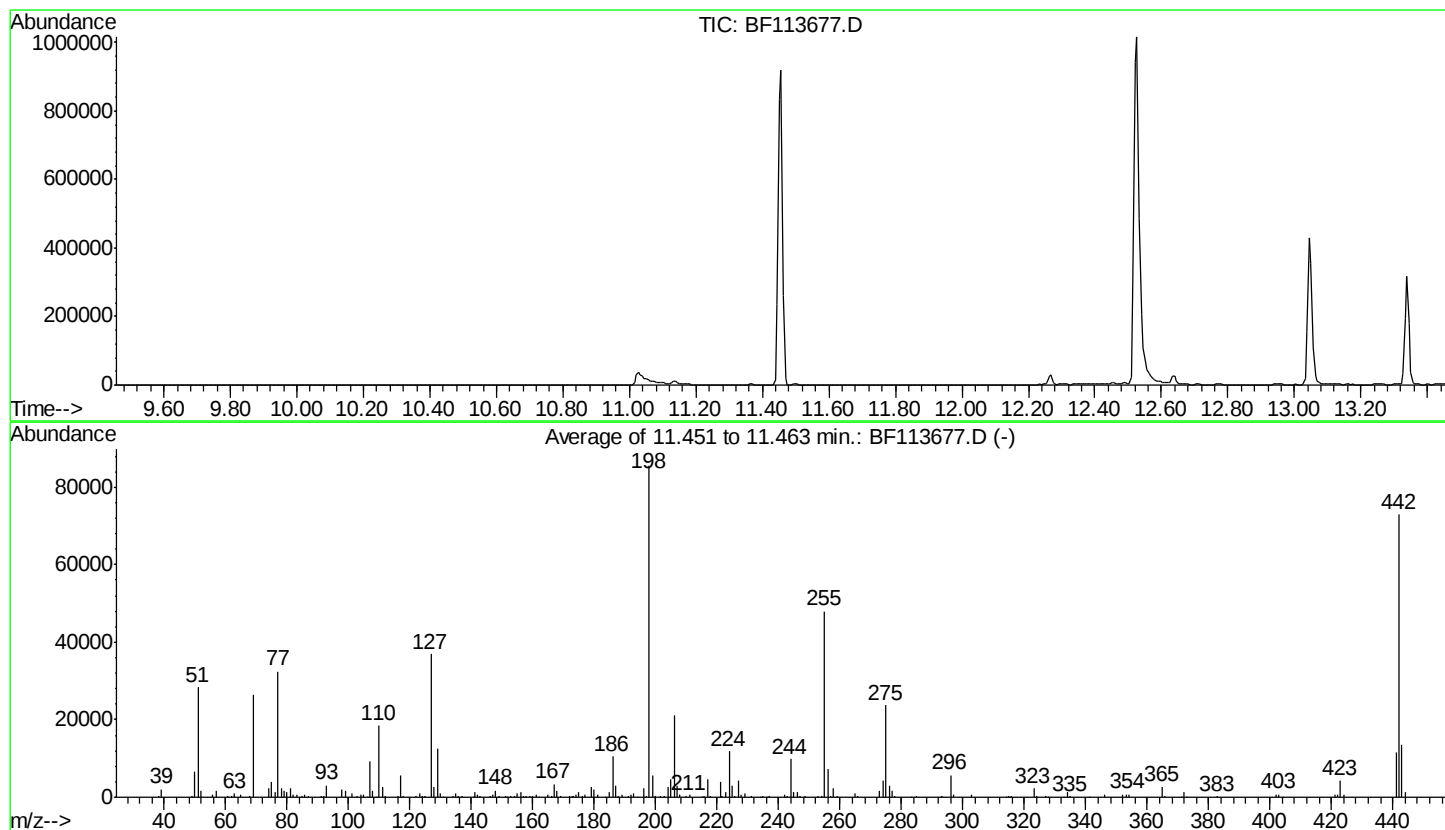

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	28260	PASS
68	69	0.00	2	1.6	427	PASS
69	198	0.00	100	30.9	26458	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	36989	PASS
197	198	0.00	2	0.5	461	PASS
198	198	100	100	100.0	85568	PASS
199	198	5	9	6.7	5734	PASS
275	198	10	60	27.7	23678	PASS
365	198	1	100	3.3	2785	PASS
441	198	0.01	100	13.4	11431	PASS
442	198	50	100	85.1	72861	PASS
443	442	15	24	18.7	13625	PASS