


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041015\
 Data File : BF078400.D
 Acq On : 10 Apr 2015 14:42
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 09 11:29:31 2015

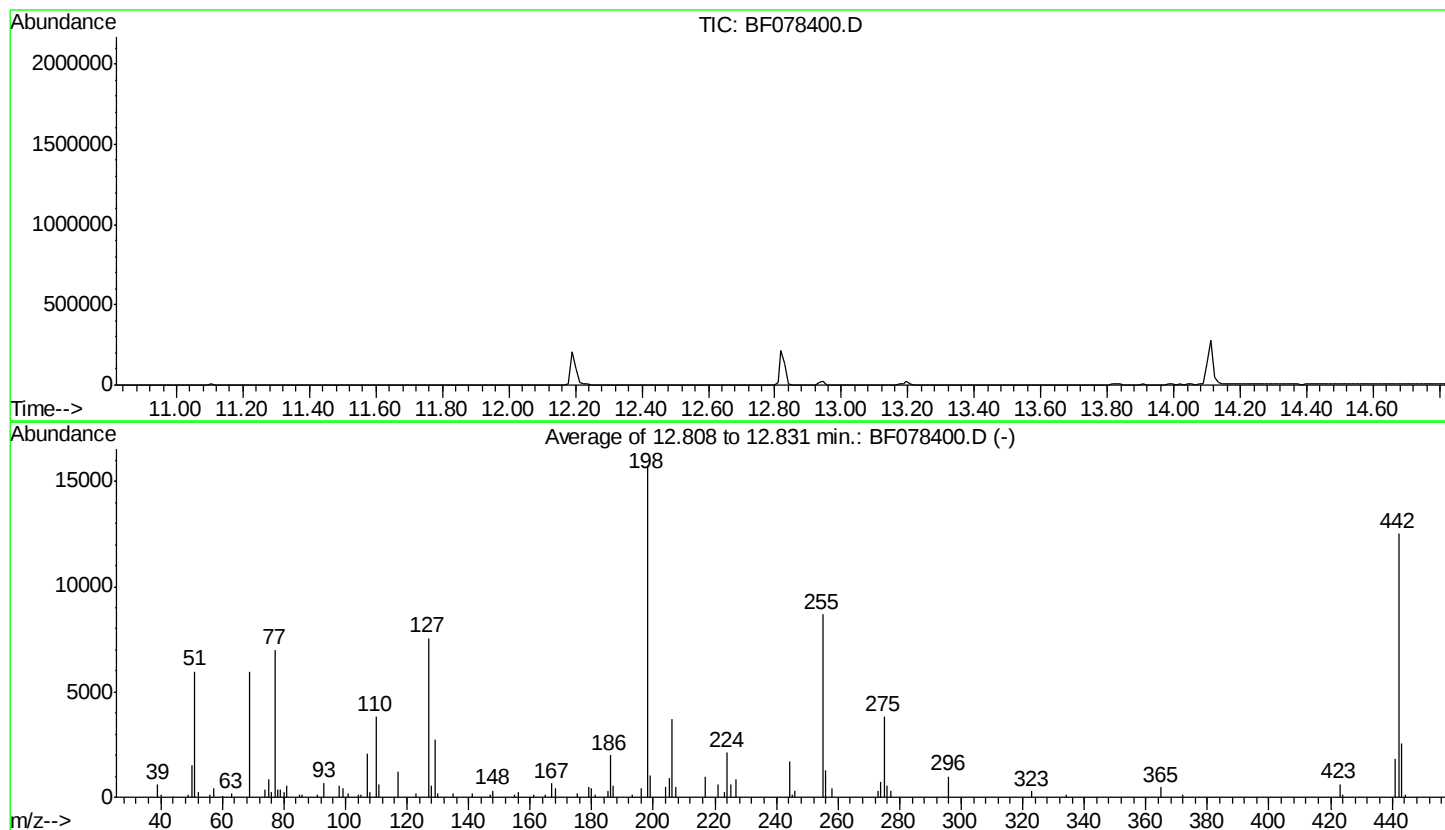

AutoFind: Scans 1043, 1044, 1045; Background Corrected with Scan 1040

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	5983	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.8	5945	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	7542	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15748	PASS
199	198	5	9	6.6	1039	PASS
275	198	10	60	24.3	3822	PASS
365	198	1	100	3.0	468	PASS
441	442	0.01	24	14.7	1839	PASS
442	198	50	100	79.5	12519	PASS
443	442	15	24	20.3	2541	PASS