


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
 Data File : BF078421.D
 Acq On : 11 Apr 2015 3:38
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 09 11:29:31 2015

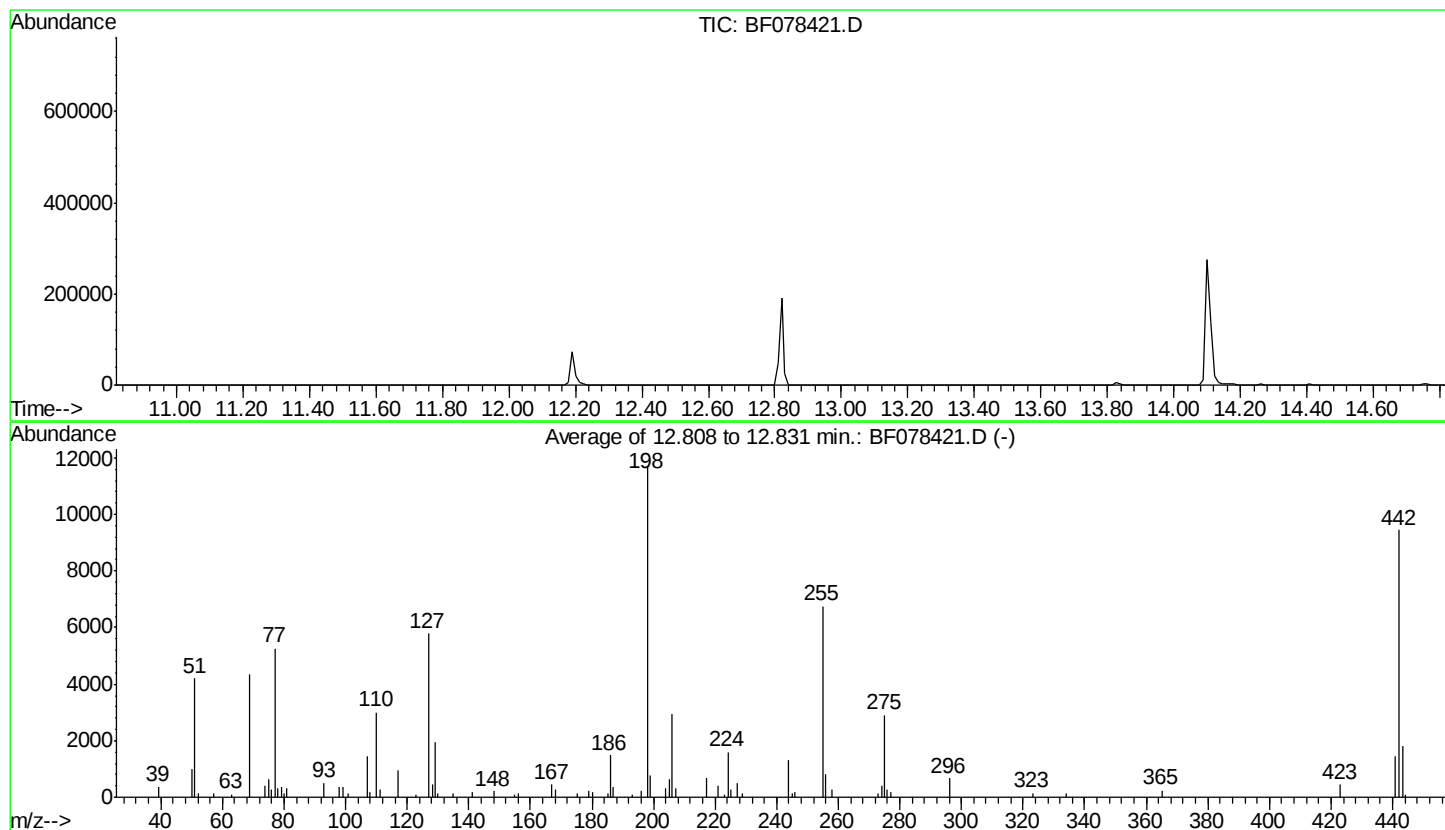

AutoFind: Scans 1043, 1044, 1045; Background Corrected with Scan 1040

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	4193	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.9	4327	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	5789	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11727	PASS
199	198	5	9	6.7	780	PASS
275	198	10	60	24.8	2906	PASS
365	198	1	100	2.0	235	PASS
441	442	0.01	24	15.6	1470	PASS
442	198	50	100	80.5	9443	PASS
443	442	15	24	19.1	1805	PASS