
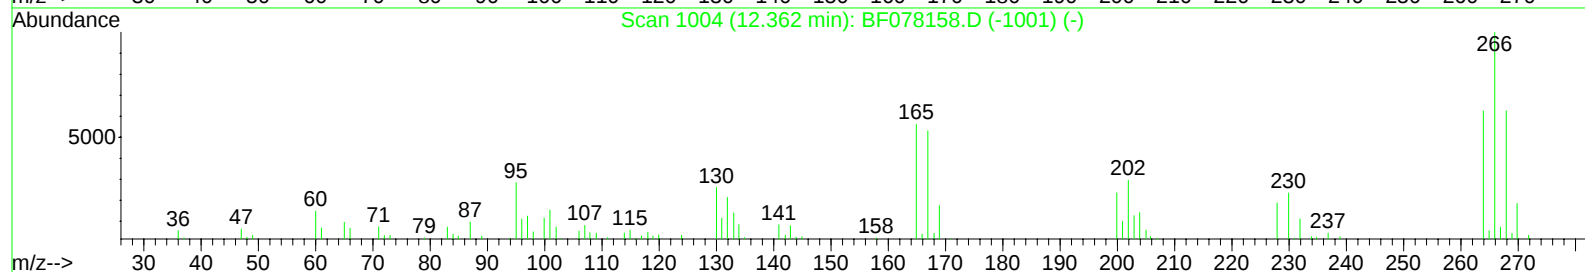
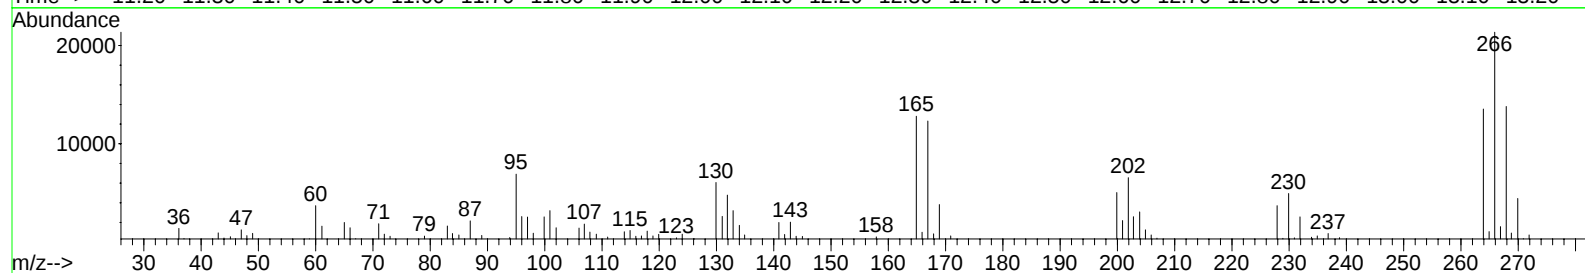


Data Path : Z:\HPCHEM1\BNA F\Data\BF041015\
Data File : BF078400.D
Acq On : 10 Apr 2015 14:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:12:28 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 09 11:29:31 2015
Response via : Initial Calibration

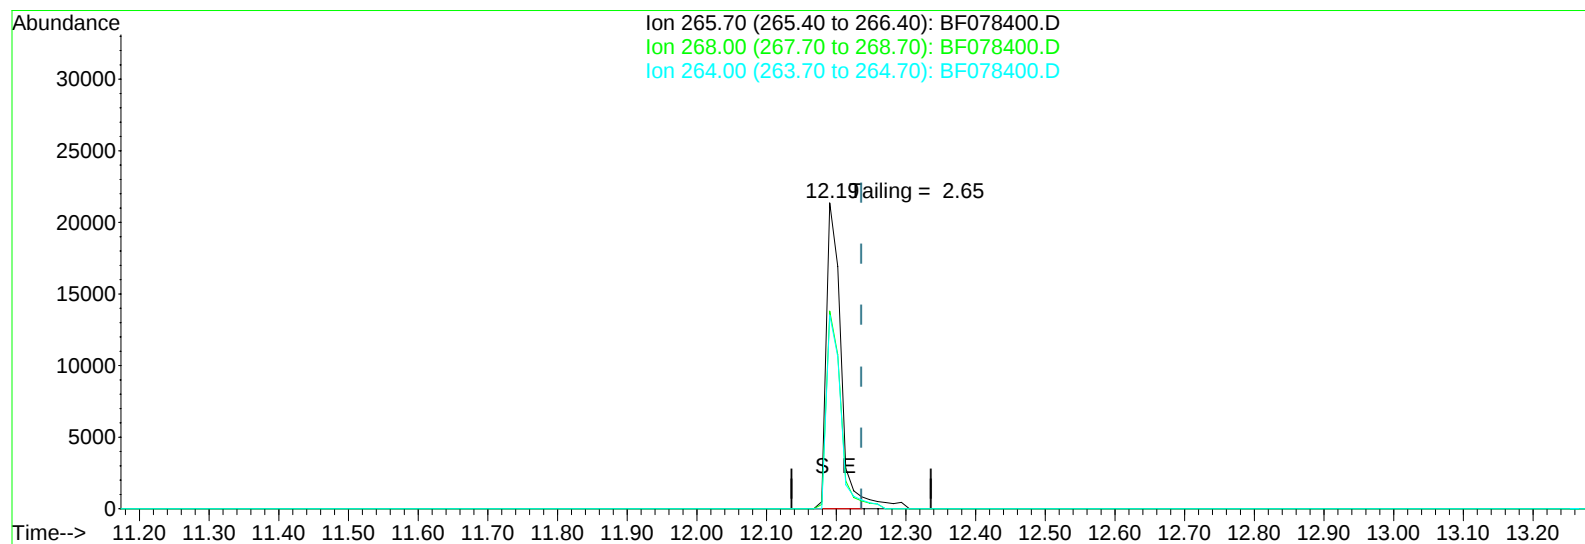

TIC: BF078400.D

(69) Pentachlorophenol (C)




12.191min (-0.045) 0.00ng m

response 29956

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	64.62
264.00	62.50	63.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF041015\
Data File : BF078400.D
Acq On : 10 Apr 2015 14:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:12:28 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 09 11:29:31 2015
Response via : Initial Calibration

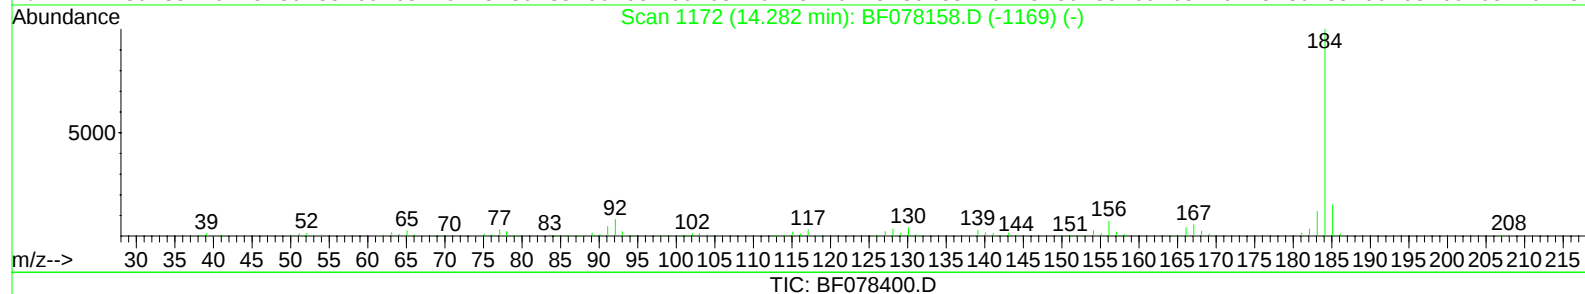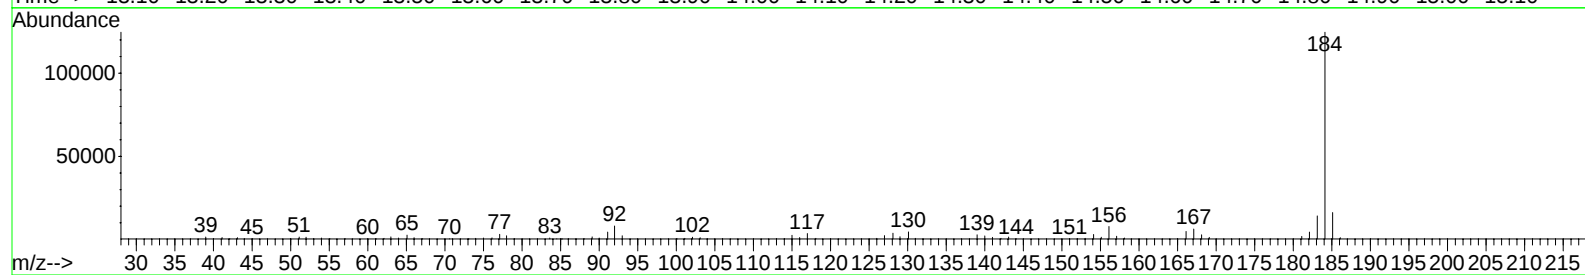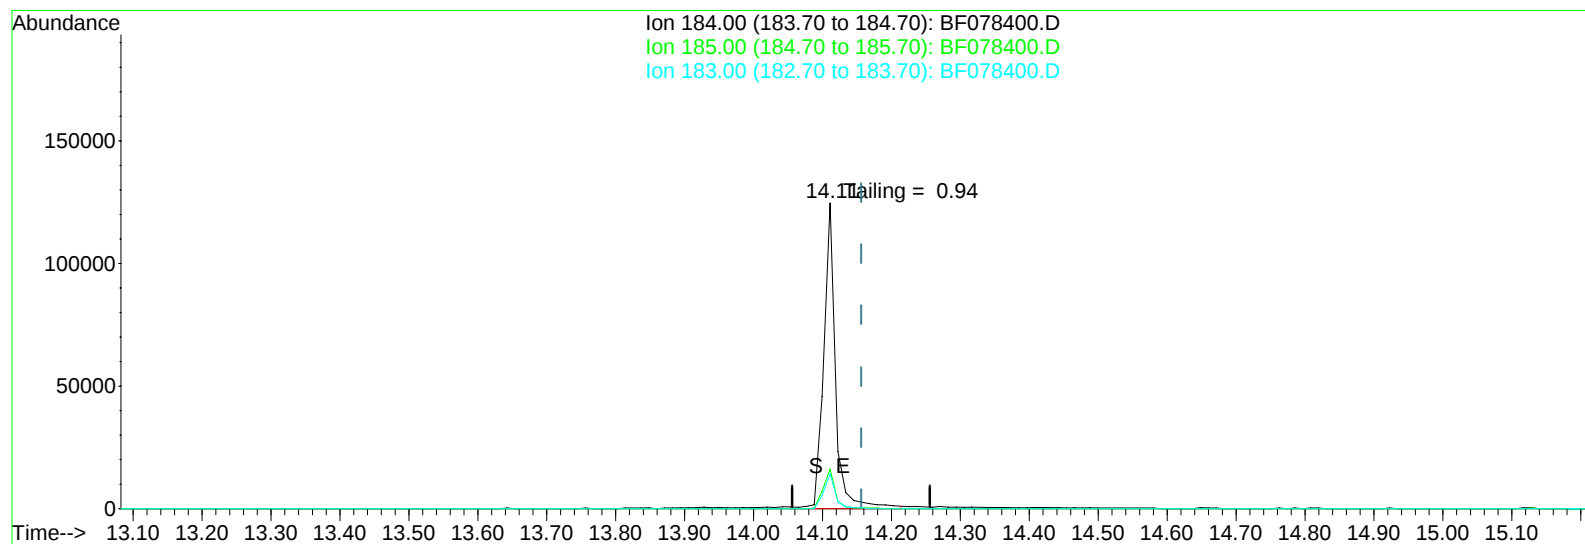

(76) Benzidine

14.111min (-0.045) 0.00ng

response 139901

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	12.97
183.00	11.90	11.39
0.00	0.00	0.00