

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
 Data File : BF078437.D
 Acq On : 11 Apr 2015 11:47
 Operator : TP/IZ
 Sample : G1793-16
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-8D

Manual Integrations
 APPROVED

apatel
 4/13/2015 4:18:46 PM

Quant Time: Apr 13 04:08:48 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 13 02:33:18 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	39673	20.00	ng	0.01
21) Naphthalene-d8	8.44	136	168457	20.00	ng	0.00
38) Acenaphthene-d10	10.59	164	87467	20.00	ng	0.00
63) Phenanthrene-d10	12.42	188	176795	20.00	ng	0.00
75) Chrysene-d12	15.69	240	189149	20.00	ng	0.01
86) Perylene-d12	17.36	264	198679	20.00	ng	0.05

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.12	112	202815	84.29	ng	0.01
7) Phenol-d6	6.46	99	270906	89.84	ng	0.01
23) Nitrobenzene-d5	7.56	82	157418	56.64	ng	0.00
41) 2,4,6-Tribromophenol	11.57	330	72421	99.83	ng	0.01
44) 2-Fluorobiphenyl	9.78	172	310618	50.76	ng	0.00
78) Terphenyl-d14	14.42	244	371105	44.33	ng	0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	6.48	94	8563	2.37	ng	82
31) Naphthalene	8.46	128	214036	24.41	ng	99
37) 2-Methylnaphthalene	9.32	142	36623	6.15	ng	97
45) 1,1'-Biphenyl	9.90	154	24925	3.48	ng	100
48) Acenaphthylene	10.42	152	37933	4.17	ng	96
49) Dimethylphthalate	10.29	163	23473	3.57	ng	99
51) Acenaphthene	10.64	154	189190	36.97	ng	99
54) Dibenzofuran	10.85	168	154503	19.77	ng	94
57) Fluorene	11.28	166	153154	24.17	ng	98
70) Phenanthrene	12.45	178	1240389	121.29	ng	98
71) Anthracene	12.51	178	228161	22.64	ng	98
72) Carbazole	12.73	167	101885	10.79	ng	99
74) Fluoranthene	13.93	202	1641101	152.16	ng	95
77) Pyrene	14.20	202	1533988	129.19	ng	95
80) Benzo(a)anthracene	15.68	228	780745	69.38	ng	96
82) Chrysene	15.72	228	580878	54.94	ng	97
85) Indeno(1,2,3-cd)pyrene	18.58	276	407153m	33.93	ng	
87) Benzo(b)fluoranthene	16.93	252	965008m	78.59	ng	
88) Benzo(k)fluoranthene	16.96	252	183161m	16.79	ng	
89) Benzo(a)pyrene	17.30	252	712966	66.53	ng	95
90) Dibenzo(a,h)anthracene	18.59	278	82491	7.69	ng	# 91
91) Benzo(g,h,i)perylene	18.95	276	390001	36.26	ng	# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
Data File : BF078437.D
Acq On : 11 Apr 2015 11:47
Operator : TP/IZ
Sample : G1793-16
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
SB-8D

Manual Integrations
APPROVED

apatel
4/13/2015 4:18:46 PM

Quant Time: Apr 13 04:08:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 13 02:33:18 2015
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.86 min Scan# 523
 Delta R.T. 0.01 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Instrument :
 BNA_F
 ClientSampleId :
 SB-8D

Tgt Ion	Ratio	Lower	Upper
152	100		
150	153.9	125.9	188.9
115	55.0	52.7	79.1




Manual Integrations
 APPROVED

apatel
 4/13/2015 4:18:46 PM

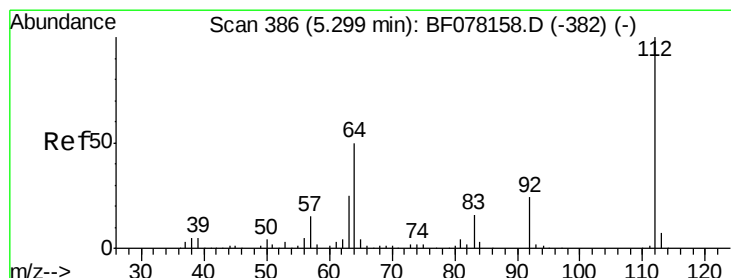

#5
 2-Fluorophenol
 Concen: 84.29 ng
 RT: 5.12 min Scan# 370
 Delta R.T. 0.01 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.0	39.9	59.9
63	30.0	20.2	30.4





#7

Phenol-d6

Concen: 89.84 ng

RT: 6.46 min Scan# 488

Delta R.T. 0.01 min

Lab File: BF078437.D

Acq: 11 Apr 2015 11:47

Instrument :

BNA_F

ClientSampleId :

SB-8D

Tgt Ion: 99 Resp: 270906

Ion Ratio Lower Upper

99 100


42 13.7 14.8 22.2#

71 27.9 26.6 39.8

Manual Integrations
APPROVED

apatel




4/13/2015 4:18:46 PM



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



#10

Phenol

Concen: 2.37 ng

RT: 6.48 min Scan# 489

Delta R.T. 0.00 min

Lab File: BF078437.D

Acq: 11 Apr 2015 11:47


Tgt Ion: 94 Resp: 8563

Ion Ratio Lower Upper

94 100

65 33.5 4.9 44.9



66 44.1 13.8 53.8



Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0









#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.44 min Scan# 661
Delta R.T. 0.00 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Instrument :
BNA_F
ClientSampled :
SB-8D

Tgt Ion	Ratio	Resp	Lower	Upper
136	100	168457		
137	10.5	9.0	13.4	
54	5.9	7.0	10.6	
68	4.7	5.4	8.2	




Manual Integrations
APPROVED


apatel
4/13/2015 4:18:46 PM



#23
Nitrobenzene-d5
Concen: 56.64 ng
RT: 7.56 min Scan# 584
Delta R.T. 0.00 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Resp	Lower	Upper
82	100	157418		
128	46.2	31.8	47.8	
54	48.7	41.5	62.3	









#31
Naphthalene
Concen: 24.41 ng
RT: 8.46 min Scan# 663
Delta R.T. 0.00 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Instrument :
BNA_F
ClientSampleId :
SB-8D

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	214036		
129	10.6	8.6	12.8	
127	12.8	10.7	16.1	




Manual Integrations
APPROVED


apatel
4/13/2015 4:18:46 PM



#37
2-Methylnaphthalene
Concen: 6.15 ng
RT: 9.32 min Scan# 738
Delta R.T. 0.00 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	36623		
141	91.1	70.3	105.5	
115	31.8	24.6	37.0	









#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.59 min Scan# 849
 Delta R.T. 0.00 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Instrument :
 BNA_F
 ClientSampled :
 SB-8D

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.2	82.2	123.2
160	44.2	34.7	52.1




Manual Integrations
 APPROVED


apatel
 4/13/2015 4:18:46 PM



#41
 2,4,6-Tribromophenol
 Concen: 99.83 ng
 RT: 11.57 min Scan# 935
 Delta R.T. 0.01 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.7	78.6	117.8
141	38.7	31.2	46.8









#44
 2-Fluorobiphenyl
 Concen: 50.76 ng
 RT: 9.78 min Scan# 778
 Delta R.T. 0.00 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Instrument :
 BNA_F
 ClientSampleId :
 SB-8D

Tgt Ion	Ratio	Resp Lower	Resp Upper
172	100		
171	35.0	28.6	42.8
170	22.9	18.5	27.7




Manual Integrations
 APPROVED


apatel
 4/13/2015 4:18:46 PM



#45
 1,1'-Biphenyl
 Concen: 3.48 ng
 RT: 9.90 min Scan# 789
 Delta R.T. 0.00 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Resp Lower	Resp Upper
154	100		
153	40.1	20.0	60.0
76	11.0	0.0	30.6





#48

Acenaphthylene

Concen: 4.17 ng

RT: 10.42 min Scan# 834

Delta R.T. 0.00 min

Lab File: BF078437.D


Acq: 11 Apr 2015 11:47

Instrument :

BNA_F

ClientSampled :




SB-8D



Tgt Ion:	152	Resp:	37933
Ion Ratio	Lower	Upper	
152	100		
151	20.8	15.7	23.5
153	15.0	10.2	15.2

Manual Integrations
APPROVED

apatel
4/13/2015 4:18:46 PM



#49

Dimethylphthalate


Concen: 3.57 ng

RT: 10.29 min Scan# 823



Delta R.T. 0.00 min


Lab File: BF078437.D

Acq: 11 Apr 2015 11:47



Tgt Ion:	163	Resp:	23473
Ion Ratio	Lower	Upper	
163	100		
194	3.3	2.3	3.5
164	11.2	8.6	13.0





#51

Acenaphthene

Concen: 36.97 ng

RT: 10.64 min Scan# 853

Delta R.T. 0.00 min

Lab File: BF078437.D


Acq: 11 Apr 2015 11:47

Instrument :

BNA_F

ClientSampleId :




SB-8D



Tgt Ion:	154	Resp:	189190
Ion Ratio	Lower	Upper	
154	100		
153	113.1	91.4	137.2
152	52.6	43.0	64.6

Manual Integrations
APPROVED

apatel
4/13/2015 4:18:46 PM



#54

Dibenzofuran


Concen: 19.77 ng

RT: 10.85 min Scan# 872



Delta R.T. 0.01 min


Lab File: BF078437.D

Acq: 11 Apr 2015 11:47



Tgt Ion:	168	Resp:	154503
Ion Ratio	Lower	Upper	
168	100		
139	34.0	31.0	46.4
169	12.8	10.7	16.1





#57

Fluorene

Concen: 24.17 ng

RT: 11.28 min Scan# 909

Delta R.T. 0.01 min

Lab File: BF078437.D

Acq: 11 Apr 2015 11:47

Instrument :

BNA_F

ClientSampleId :





SB-8D

Manual Integrations
APPROVED

apatel

4/13/2015 4:18:46 PM

Tgt Ion:	166	Resp:	153154
Ion Ratio	Lower	Upper	
166	100		
165	100.3	78.9	118.3
167	13.7	10.7	16.1



#63

Phenanthrene-d10

Concen: 20.00 ng




RT: 12.42 min Scan# 1009


Delta R.T. 0.00 min

Lab File: BF078437.D

Acq: 11 Apr 2015 11:47

Tgt Ion:	188	Resp:	176795
Ion Ratio	Lower	Upper	
188	100		
94	10.2	9.0	13.4
80	10.8	9.5	14.3






#70
Phenanthrene
Concen: 121.29 ng
RT: 12.45 min Scan# 1012
Delta R.T. 0.01 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Instrument :
BNA_F
ClientSampled :
SB-8D




Tgt Ion:178 Resp: 1240389
Ion Ratio Lower Upper
178 100
176 19.9 15.4 23.0
179 16.1 12.2 18.2

Manual Integrations
APPROVED

apatel
4/13/2015 4:18:46 PM





Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E




#71
Anthracene
Concen: 22.64 ng
RT: 12.51 min Scan# 1017
Delta R.T. 0.00 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Tgt Ion:178 Resp: 228161
Ion Ratio Lower Upper
178 100
176 17.8 14.8 22.2
179 17.0 12.4 18.6

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E









#72
 Carbazole
 Concen: 10.79 ng
 RT: 12.73 min Scan# 1036
 Delta R.T. 0.00 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Instrument :
 BNA_F
 ClientSampleId :
 SB-8D

Tgt Ion	Ratio	Lower	Upper
167	100		
166	20.8	16.8	25.2
139	12.0	10.0	15.0




Manual Integrations
 APPROVED


apatel
 4/13/2015 4:18:46 PM



#74
 Fluoranthene
 Concen: 152.16 ng
 RT: 13.93 min Scan# 1141
 Delta R.T. 0.02 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.6	0.0	35.2
203	18.3	0.0	38.5





#75

Chrysene-d12

Concen: 20.00 ng

RT: 15.69 min Scan# 1295

Delta R.T. 0.01 min

Lab File: BF078437.D

Acq: 11 Apr 2015 11:47

Instrument :

BNA_F


ClientSampled :

SB-8D

Tgt Ion:	240	Resp:	189149
Ion Ratio	Lower	Upper	
240	100		
120	10.9	7.1	10.7#
236	25.7	21.4	32.2

Manual Integrations
APPROVED




apatel
4/13/2015 4:18:46 PM



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



#77

Pyrene

Concen: 129.19 ng

RT: 14.20 min Scan# 1165

Delta R.T. 0.02 min

Lab File: BF078437.D




Acq: 11 Apr 2015 11:47


Tgt Ion:	202	Resp:	1533988
Ion Ratio	Lower	Upper	
202	100		
200	22.5	16.3	24.5
203	19.7	13.8	20.6

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E









#78
 Terphenyl-d14
 Concen: 44.33 ng
 RT: 14.42 min Scan# 1184
 Delta R.T. 0.01 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Instrument :
 BNA_F
 ClientSampleId :
 SB-8D

Tgt Ion	Ratio	Resp Lower	Resp Upper
244	100		
212	5.9	5.0	7.4
122	7.3	7.1	10.7




Manual Integrations
 APPROVED


apatel
 4/13/2015 4:18:46 PM



#80
 Benzo(a)anthracene
 Concen: 69.38 ng
 RT: 15.68 min Scan# 1294
 Delta R.T. 0.01 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
226	29.1	21.3	31.9
229	20.9	15.4	23.2





#82

Chrysene

Concen: 54.94 ng

RT: 15.72 min Scan# 1298

Delta R.T. 0.01 min

Lab File: BF078437.D


Acq: 11 Apr 2015 11:47

Instrument :

BNA_F

ClientSampleId :




SB-8D



Tgt Ion:	228	Resp:	580878
Ion Ratio	Lower	Upper	
228	100		
226	30.7	24.2	36.4
229	23.2	15.8	23.8

Manual Integrations
APPROVED

apatel
4/13/2015 4:18:46 PM



#85

Indeno(1,2,3-cd)pyrene

Concen: 33.93 ng m




RT: 18.58 min Scan# 1548


Delta R.T. 0.06 min

Lab File: BF078437.D

Acq: 11 Apr 2015 11:47

Tgt Ion:	276	Resp:	407153
Ion Ratio	Lower	Upper	
276	100		
138	4.8	16.9	25.3#
277	4.6	15.8	23.6#









#86
Perylene-d12
Concen: 20.00 ng
RT: 17.36 min Scan# 1441
Delta R.T. 0.05 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Instrument :
BNA_F
ClientSampleId :
SB-8D

Tgt Ion	Ratio	Resp	Lower	Upper
264	100	198679		
260	23.1	18.6	27.8	
265	22.7	17.0	25.6	




Manual Integrations
APPROVED


apatel
4/13/2015 4:18:46 PM



#87
Benzo(b)fluoranthene
Concen: 78.59 ng m
RT: 16.93 min Scan# 1404
Delta R.T. 0.02 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	965008		
253	23.3	17.2	25.8	
125	13.1	7.0	10.4	









#88
Benzo(k)fluoranthene
Concen: 16.79 ng m
RT: 16.96 min Scan# 1406
Delta R.T. 0.02 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Instrument :
BNA_F
ClientSampleId :
SB-8D

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.5	26.3
125	13.9	11.6	17.4




Manual Integrations
APPROVED


apatel
4/13/2015 4:18:46 PM



#89
Benzo(a)pyrene
Concen: 66.53 ng
RT: 17.30 min Scan# 1436
Delta R.T. 0.05 min
Lab File: BF078437.D
Acq: 11 Apr 2015 11:47

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.9	16.8	25.2
125	10.4	7.4	11.0









#90
 Dibenzo(a,h)anthracene
 Concen: 7.69 ng
 RT: 18.59 min Scan# 1549
 Delta R.T. 0.03 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Instrument :
 BNA_F
 ClientSampleId :
 SB-8D

Tgt Ion:	278	Resp:	82491
Ion Ratio	Lower	Upper	
278	100		
139	20.3	13.6	20.4
279	28.6	19.0	28.6#

Manual Integrations
 APPROVED

apatel
 4/13/2015 4:18:46 PM



#91
 Benzo(g,h,i)perylene
 Concen: 36.26 ng
 RT: 18.95 min Scan# 1580
 Delta R.T. 0.07 min
 Lab File: BF078437.D
 Acq: 11 Apr 2015 11:47

Tgt Ion:	276	Resp:	390001
Ion Ratio	Lower	Upper	
276	100		
277	24.1	19.0	28.4
138	19.6	19.9	29.9#

