

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
 Data File : BF078405.D
 Acq On : 10 Apr 2015 17:58
 Operator : TP/IZ
 Sample : PB82775BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB82775BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.035	11	13	15	rVB	408652	492975	12.69%	3.576%
2	1.516	54	55	63	rBV	1515281	2572761	66.21%	18.661%
3	1.618	63	64	98	rVB	2000829	3885528	100.00%	28.183%
4	4.522	317	318	327	rVB	47830	81101	2.09%	0.588%
5	5.116	367	370	373	rBV	577769	656262	16.89%	4.760%
6	6.453	485	487	490	rBV	608070	638369	16.43%	4.630%
7	6.567	495	497	500	rVV	674340	692612	17.83%	5.024%
8	6.853	520	522	525	rVB	125459	145090	3.73%	1.052%
9	7.048	536	539	541	rBV	406253	536689	13.81%	3.893%
10	7.562	581	584	586	rBV	409062	416137	10.71%	3.018%
11	8.430	658	660	663	rBV	155670	194532	5.01%	1.411%
12	9.779	776	778	781	rBV	936655	853971	21.98%	6.194%
13	10.591	847	849	852	rBV	258405	230187	5.92%	1.670%
14	11.562	932	934	937	rBV2	439239	492982	12.69%	3.576%
15	12.419	1006	1009	1011	rBV	217729	241083	6.20%	1.749%
16	14.408	1181	1183	1186	rBV	1072819	1071014	27.56%	7.769%
17	15.677	1292	1294	1297	rBV	275428	287772	7.41%	2.087%
18	17.403	1442	1445	1448	rBV	252615	297486	7.66%	2.158%


Sum of corrected areas: 13786551

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
Data File : BF078405.D
Acq On : 10 Apr 2015 17:58
Operator : TP/IZ
Sample : PB82775BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82775BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

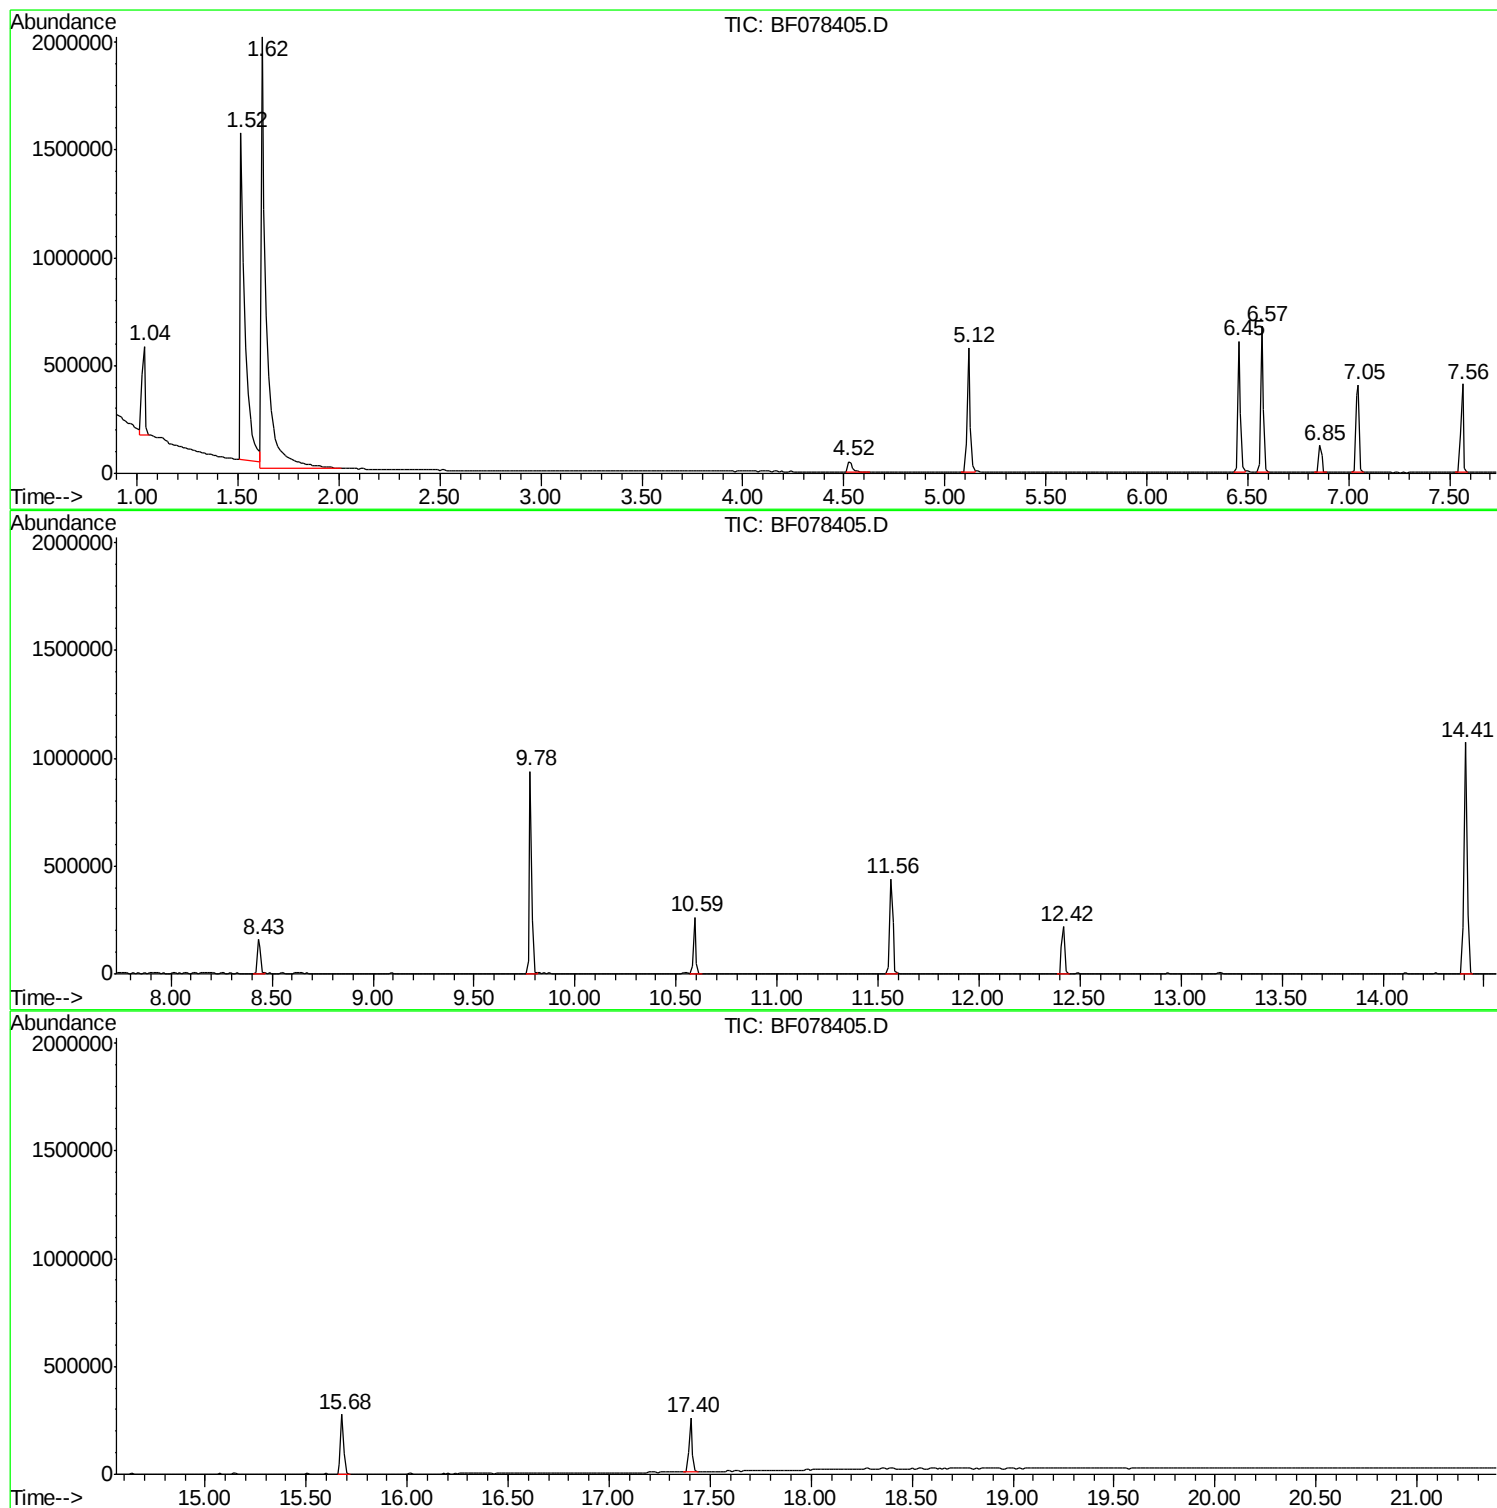

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
Data File : BF078405.D
Acq On : 10 Apr 2015 17:58
Operator : TP/IZ
Sample : PB82775BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82775BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown4.52 Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.52	11.18 ng	81101	1,4-Dichlorobenzene-d4	6.85

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42	
2	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	23	
3	5-Hexen-2-one	98	C6H10O	000109-49-9	9	
4	tert-Butyl Hydroperoxide	90	C4H10O2	000075-91-2	9	
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9	

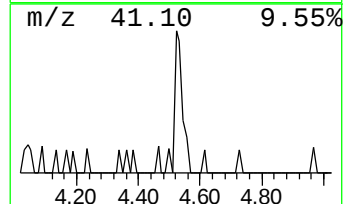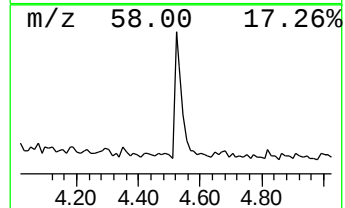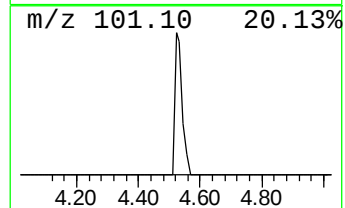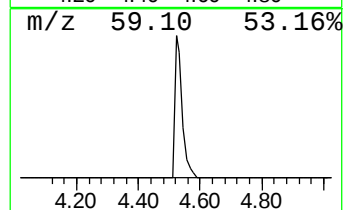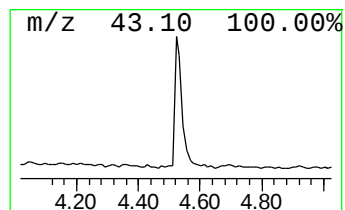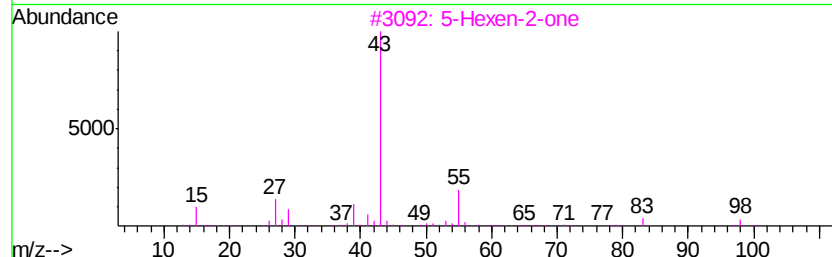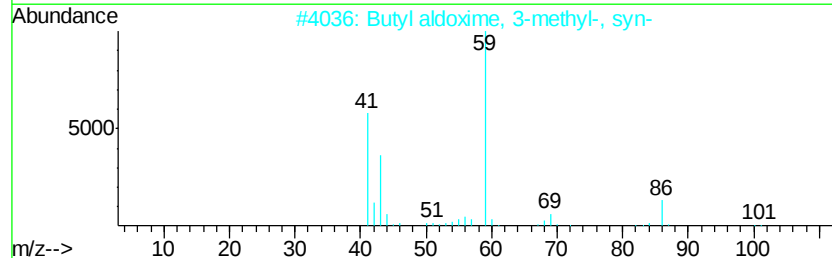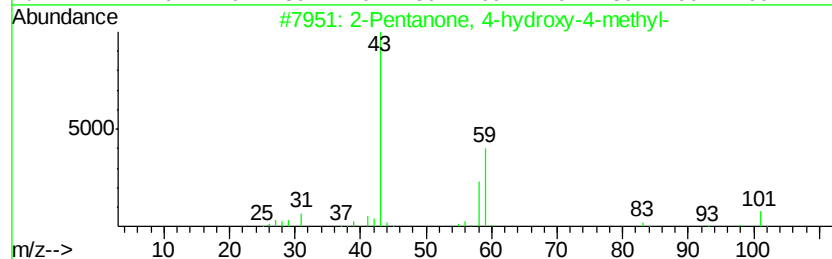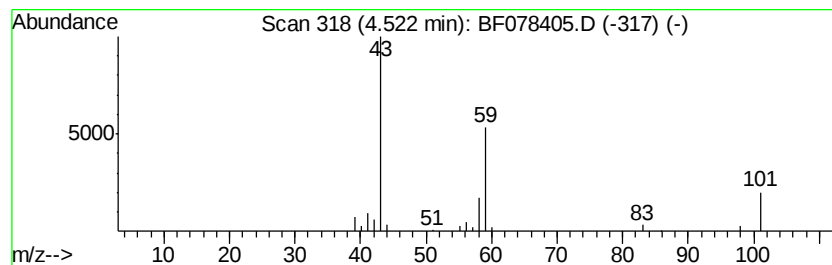

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
Data File : BF078405.D
Acq On : 10 Apr 2015 17:58
Operator : TP/IZ
Sample : PB82775BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82775BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.57 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	95.47 ng	692612	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16		
2	5-Aminoindole	132	C8H8N2	005192-03-0	12		
3	Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10		
4	Bicyclo[4.2.0]octa-1,3,5-triene, ...	132	C10H12	028749-81-7	9		
5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9		

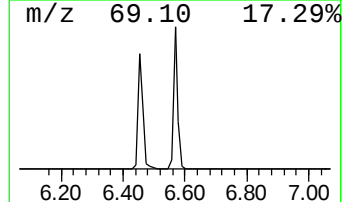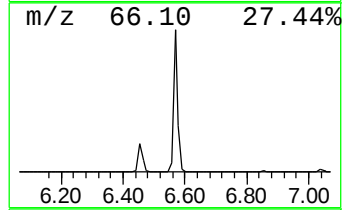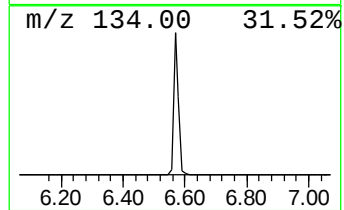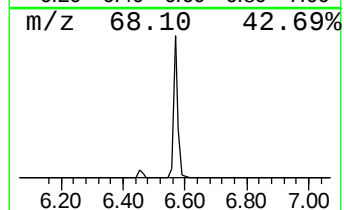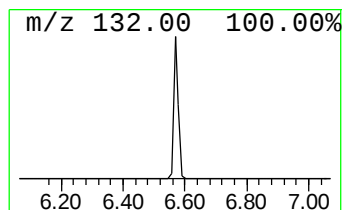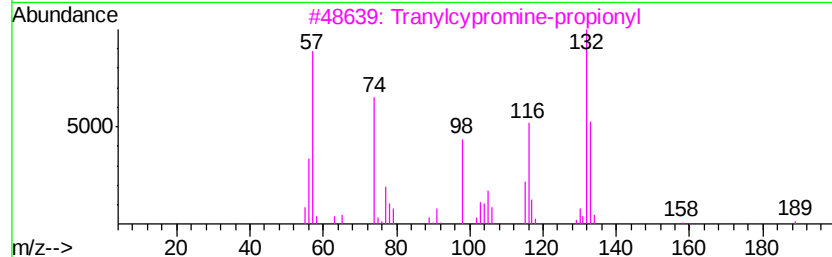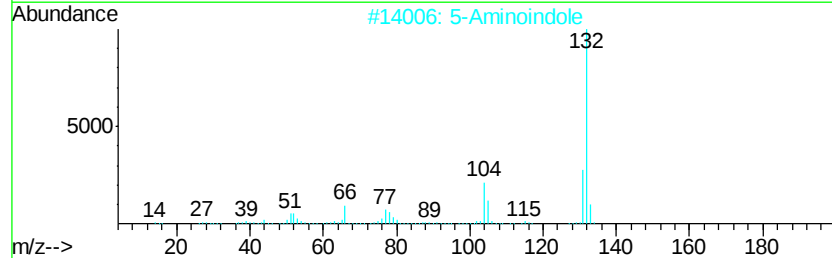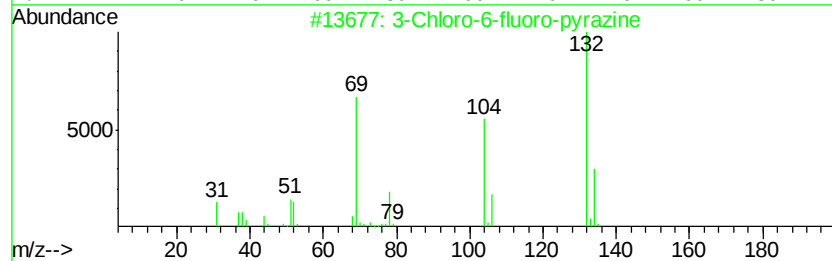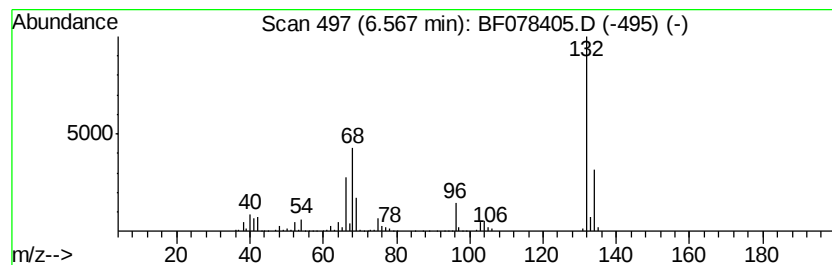

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041015\
Data File : BF078405.D
Acq On : 10 Apr 2015 17:58
Operator : TP/IZ
Sample : PB82775BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82775BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown4.52	4.52	11.2	ng	81101	1	6.85	145090	20.0
unknown6.57	6.57	95.5	ng	692612	1	6.85	145090	20.0