


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041015\
Data File : BF078421.D
Acq On : 11 Apr 2015 3:38
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 31 14:58:34 2015

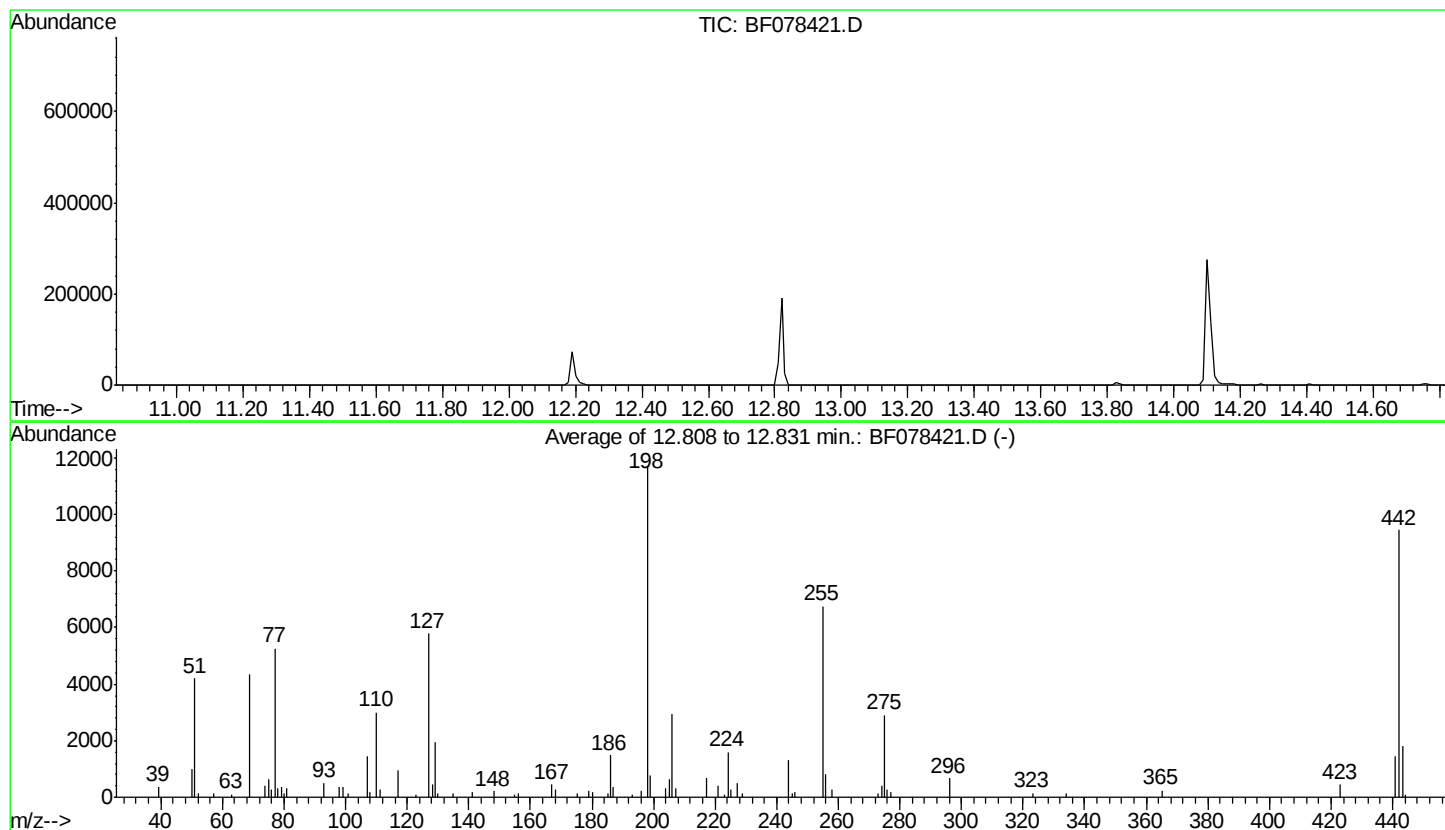

AutoFind: Scans 1043, 1044, 1045; Background Corrected with Scan 1040

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	4193	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.9	4327	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	5789	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11727	PASS
199	198	5	9	6.7	780	PASS
275	198	10	60	24.8	2906	PASS
365	198	1	100	2.0	235	PASS
441	442	0.01	24	15.6	1470	PASS
442	198	50	100	80.5	9443	PASS
443	442	15	24	19.1	1805	PASS