


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041015\
 Data File : BF078444.D
 Acq On : 11 Apr 2015 17:06
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

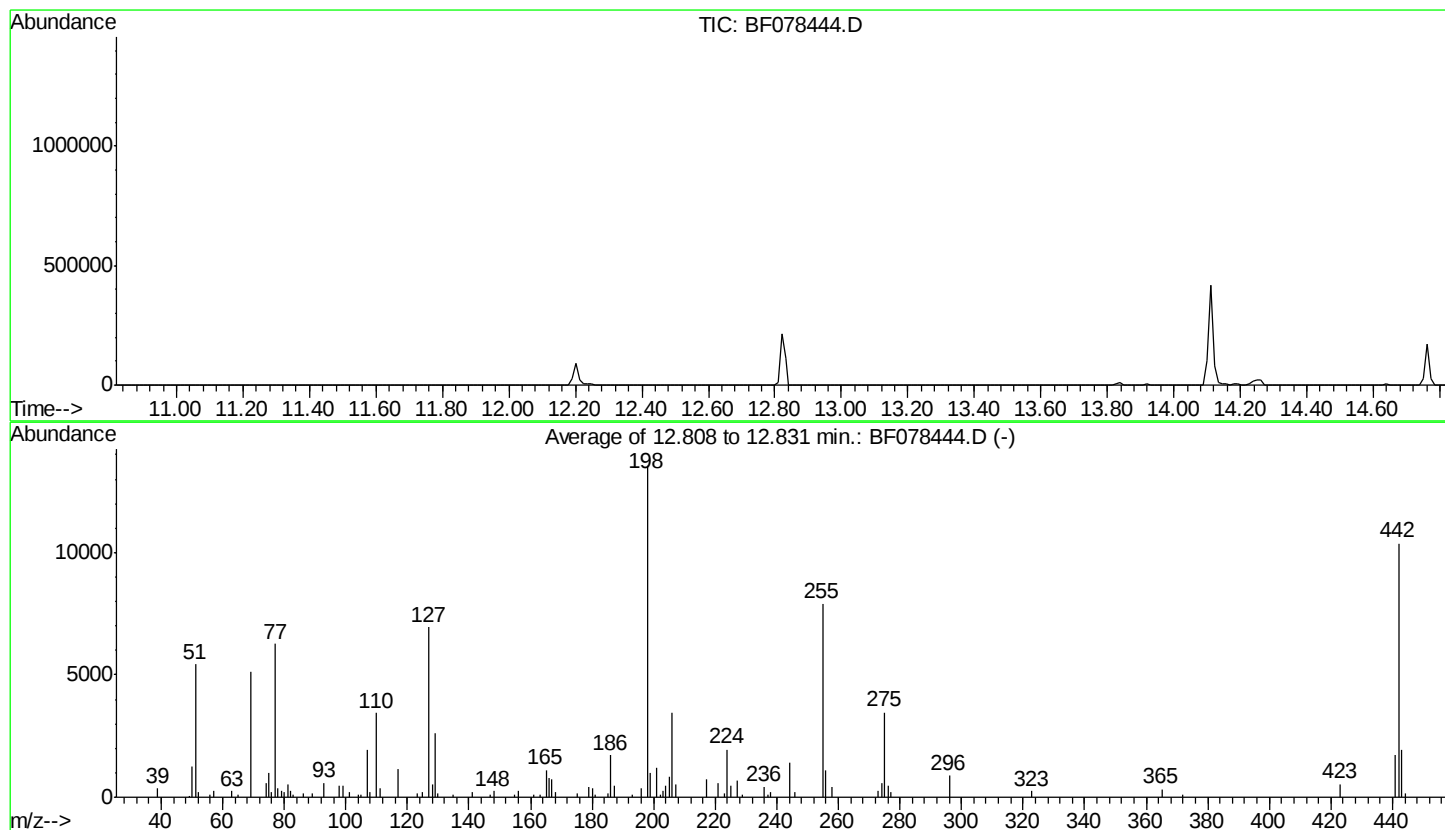

AutoFind: Scans 1043, 1044, 1045; Background Corrected with Scan 1040

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	5437	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.0	5150	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	6956	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13550	PASS
199	198	5	9	7.4	1000	PASS
275	198	10	60	25.6	3466	PASS
365	198	1	100	2.5	337	PASS
441	442	0.01	24	16.4	1707	PASS
442	198	50	100	76.6	10378	PASS
443	442	15	24	18.7	1940	PASS