
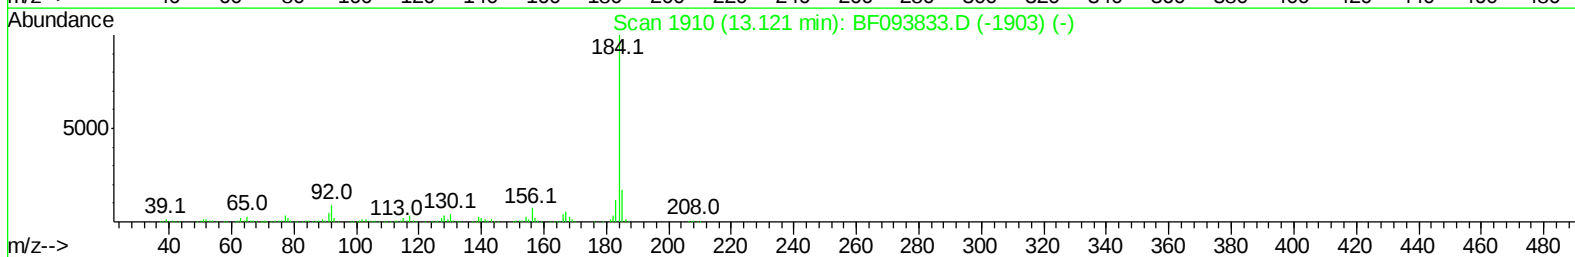
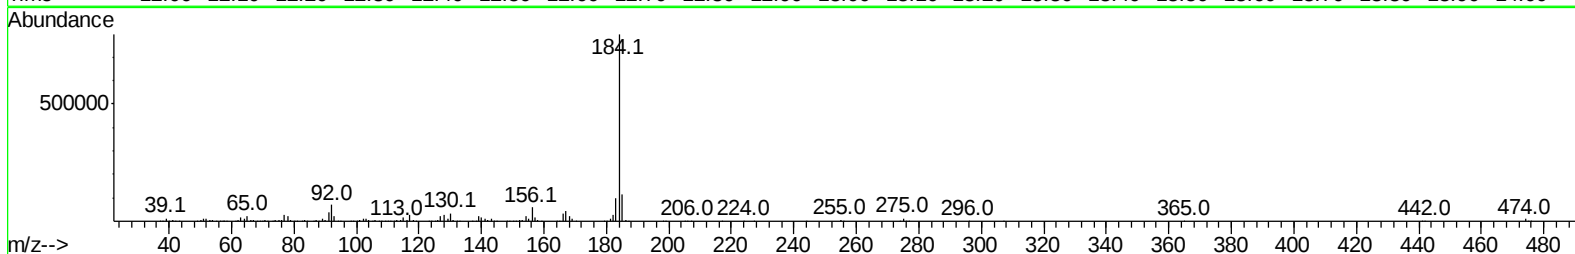


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041017\
Data File : BF094302.D
Acq On : 10 Apr 2017 10:38
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 04:43:38 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

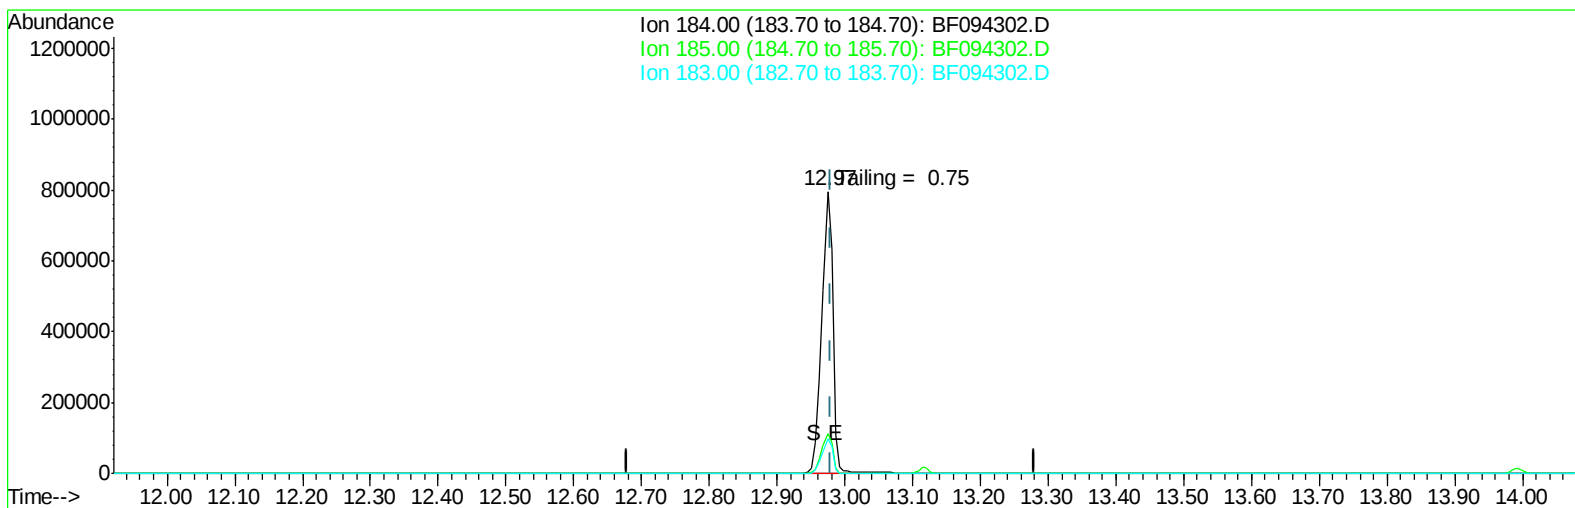

TIC: BF094302.D

(76) Benzidine




12.974min (-0.006) 99056.64ng

response 882110

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.12#
183.00	12.20	12.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041017\
Data File : BF094302.D
Acq On : 10 Apr 2017 10:38
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 04:43:38 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

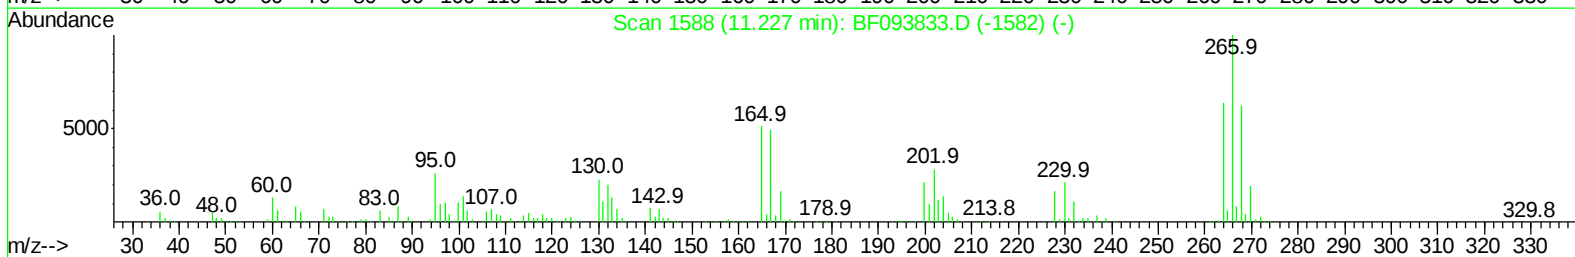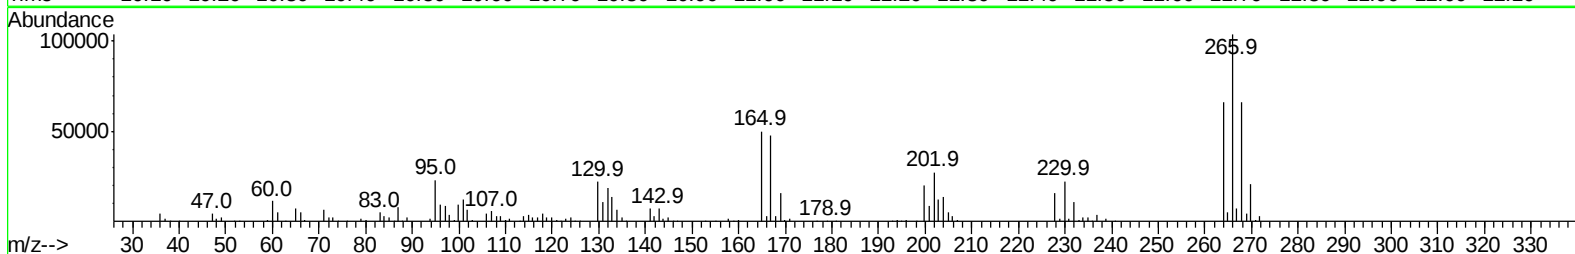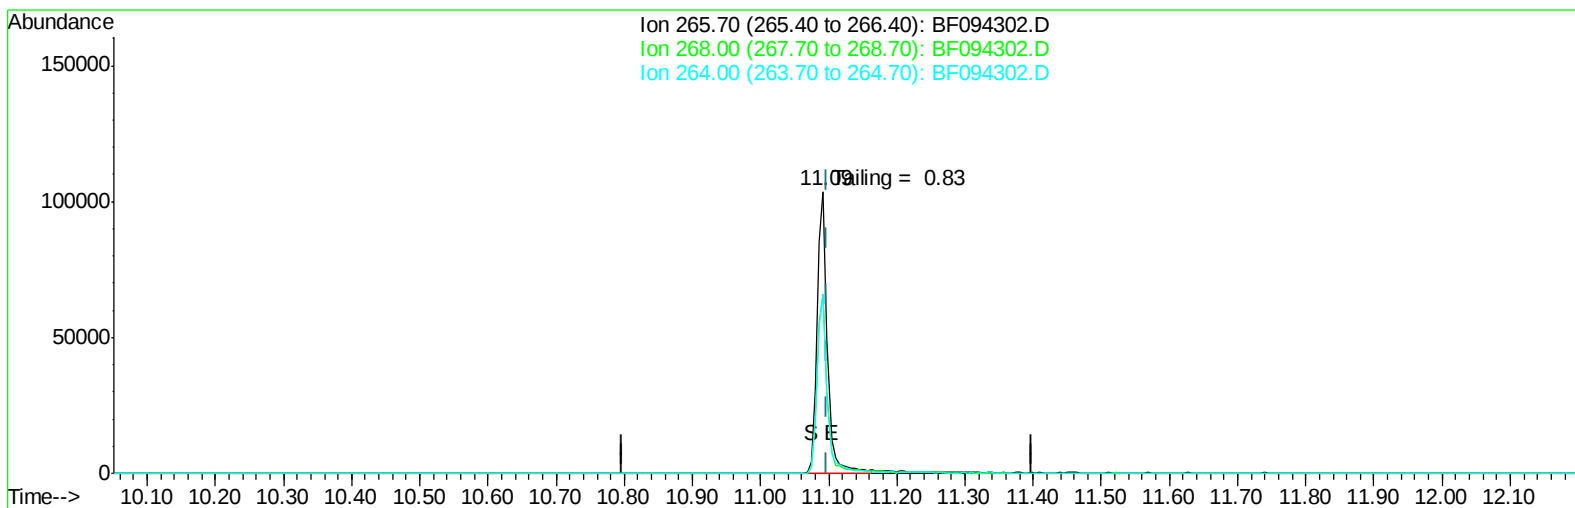

TIC: BF094302.D

(69) Pentachlorophenol (C)

11.092min (-0.006) 0.00ng

response 110980

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.61
264.00	64.60	63.55
0.00	0.00	0.00