
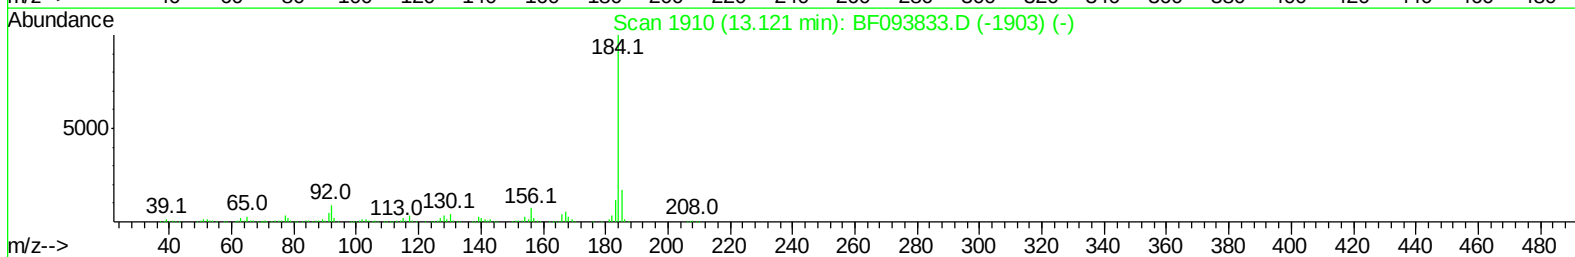
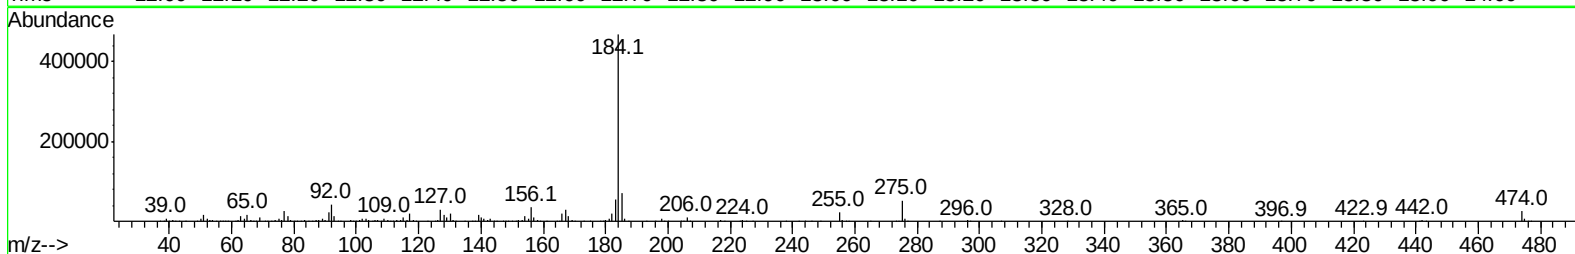


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041017\
Data File : BF094327.D
Acq On : 10 Apr 2017 23:56
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 04:47:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

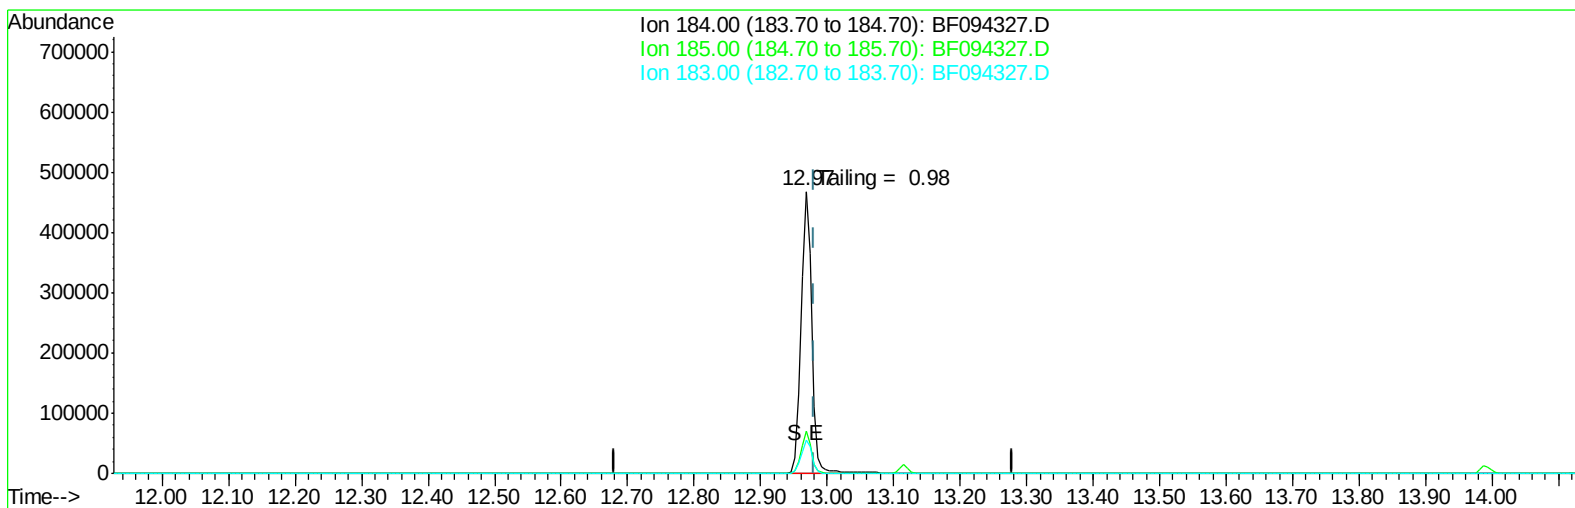

TIC: BF094327.D

(76) Benzidine




12.968min (-0.012) 0.00ng

response 535573

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.80#
183.00	12.20	11.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041017\
Data File : BF094327.D
Acq On : 10 Apr 2017 23:56
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 04:47:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

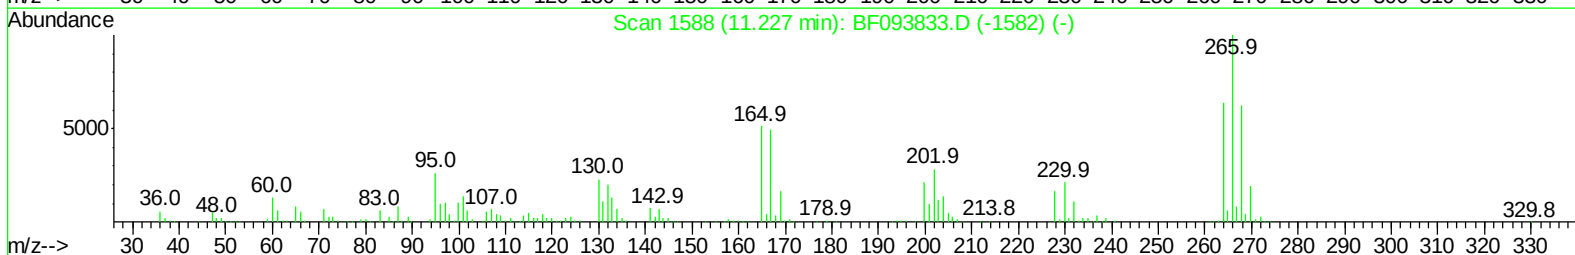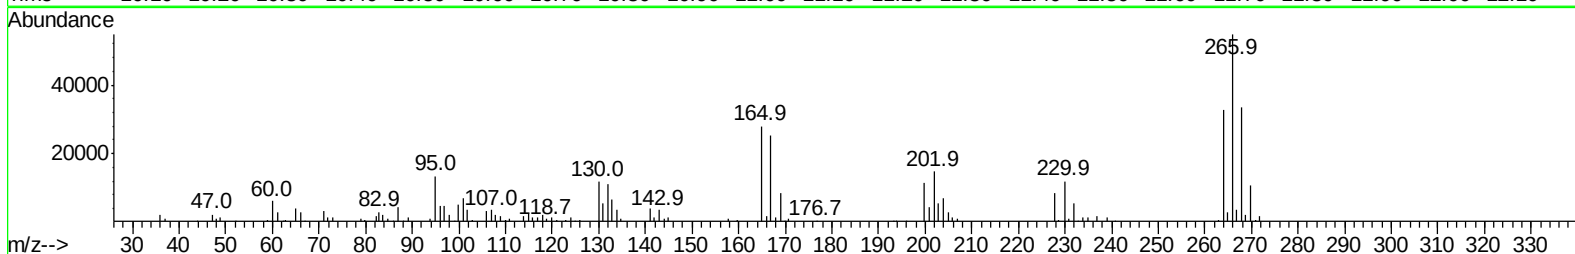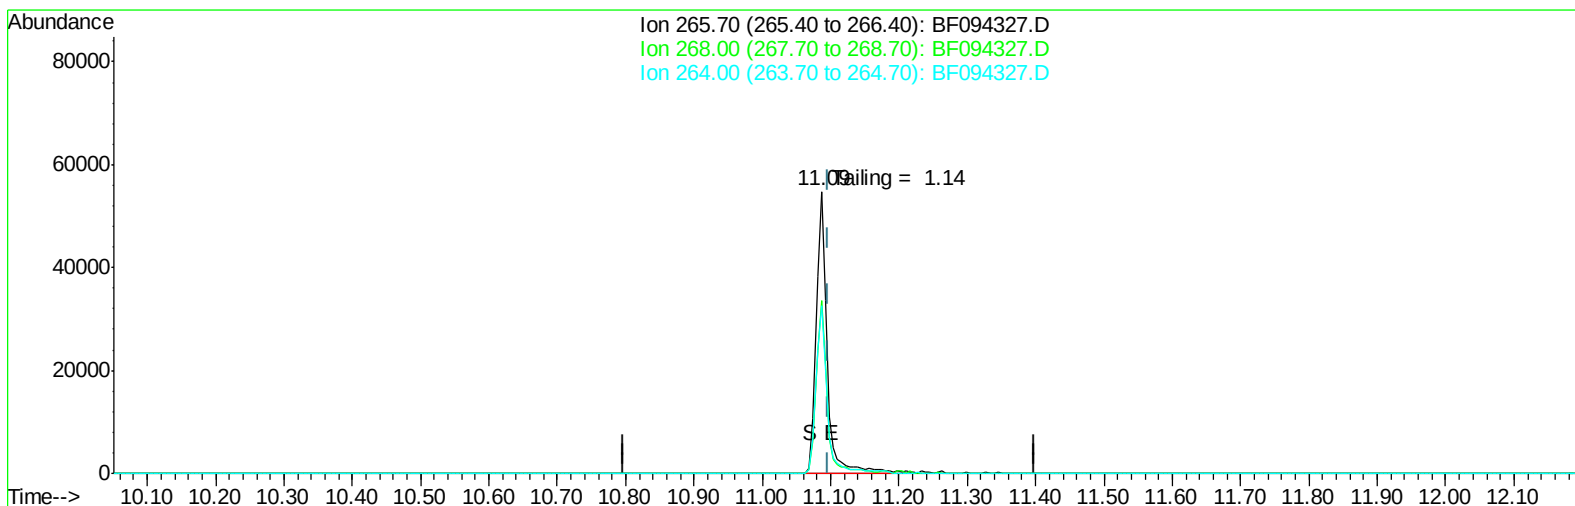

TIC: BF094327.D

(69) Pentachlorophenol (C)

11.086min (-0.012) 86959.36ng

response 60354

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.32
264.00	64.60	59.79
0.00	0.00	0.00