


Data Path : Z:\HPCHEM1\BNA F\Data\BF041017\
 Data File : BF094302.D
 Acq On : 10 Apr 2017 10:38
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 13:20:29 2017

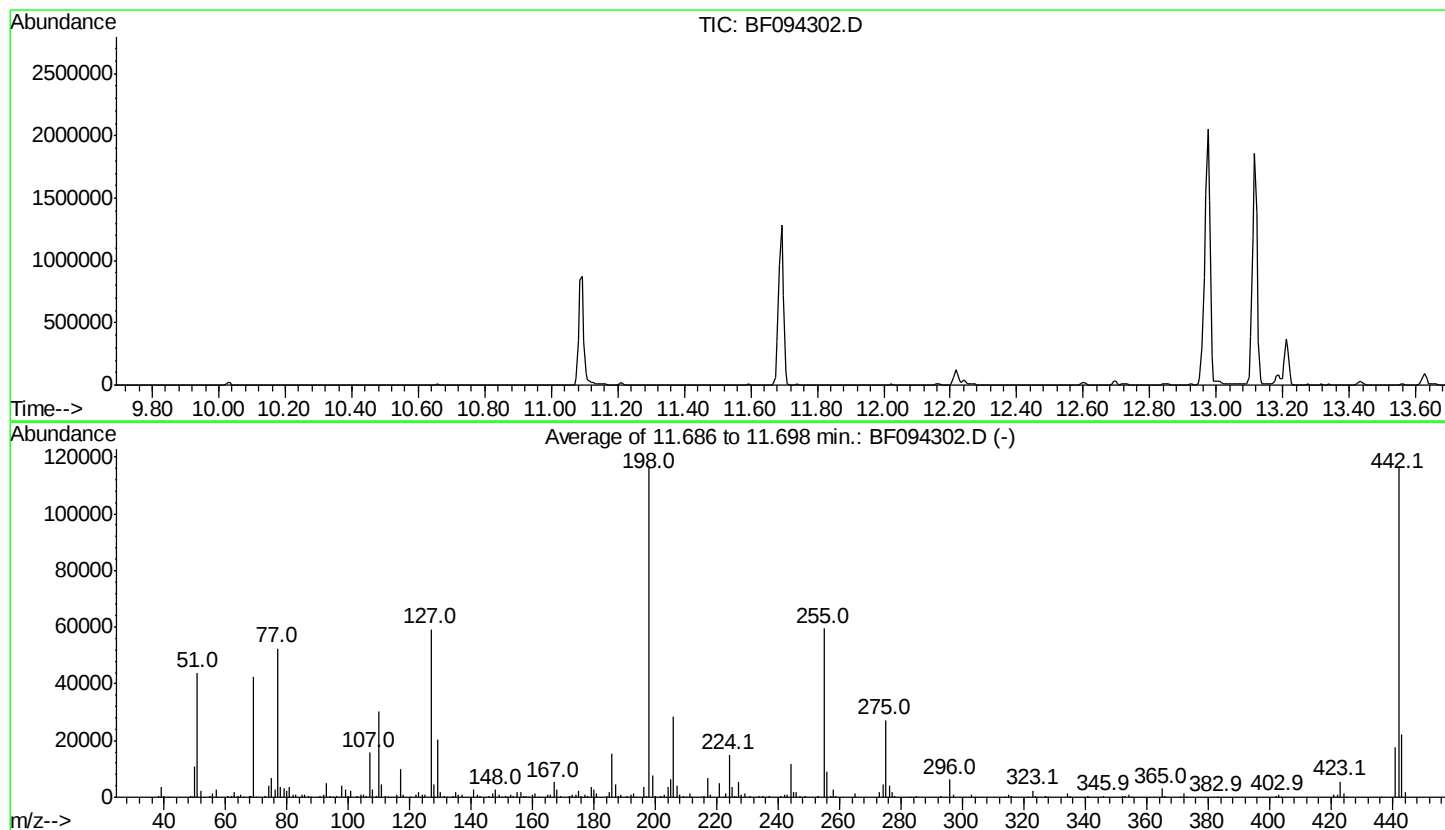

AutoFind: Scans 1666, 1667, 1668; Background Corrected with Scan 1660

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	43885	PASS
68	69	0.00	2	1.1	462	PASS
69	198	0.00	100	36.2	42376	PASS
70	69	0.00	2	0.3	143	PASS
127	198	10	80	50.7	59264	PASS
197	198	0.00	2	0.2	290	PASS
198	198	100	100	100.0	116976	PASS
199	198	5	9	6.8	7910	PASS
275	198	10	60	23.3	27218	PASS
365	198	1	100	2.6	3068	PASS
441	442	0.01	24	15.1	17674	PASS
442	198	50	100	99.8	116728	PASS
443	442	15	24	18.8	21987	PASS