


Data Path : Z:\HPCHEM1\BNA F\Data\BF041017\
 Data File : BF094327.D
 Acq On : 10 Apr 2017 23:29
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 13:20:29 2017

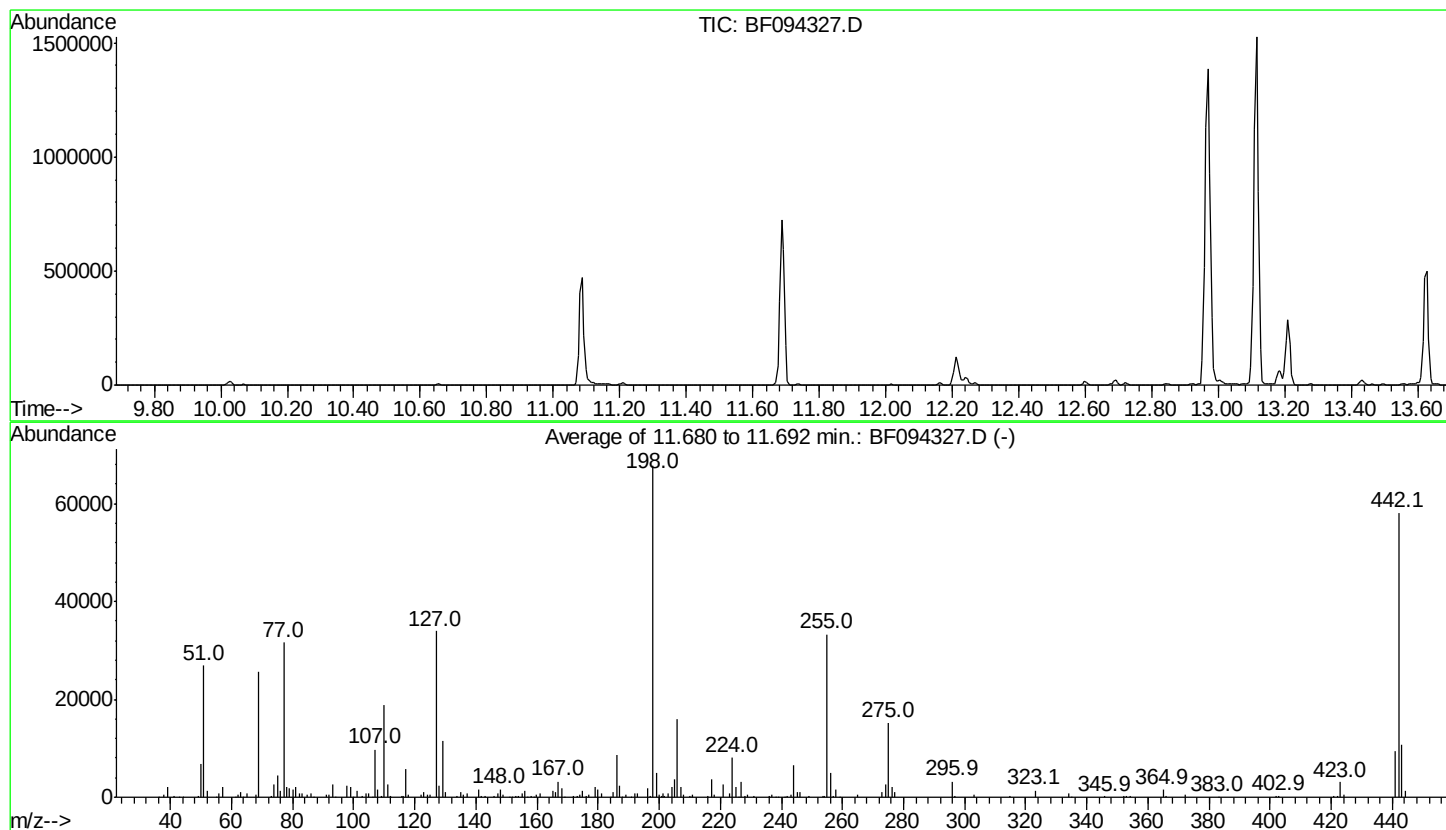

AutoFind: Scans 1665, 1666, 1667; Background Corrected with Scan 1659

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	26909	PASS
68	69	0.00	2	1.6	417	PASS
69	198	0.00	100	37.9	25680	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	33992	PASS
197	198	0.00	2	0.3	228	PASS
198	198	100	100	100.0	67797	PASS
199	198	5	9	7.2	4876	PASS
275	198	10	60	22.4	15199	PASS
365	198	1	100	2.3	1544	PASS
441	442	0.01	24	16.0	9334	PASS
442	198	50	100	85.8	58178	PASS
443	442	15	24	18.4	10712	PASS