
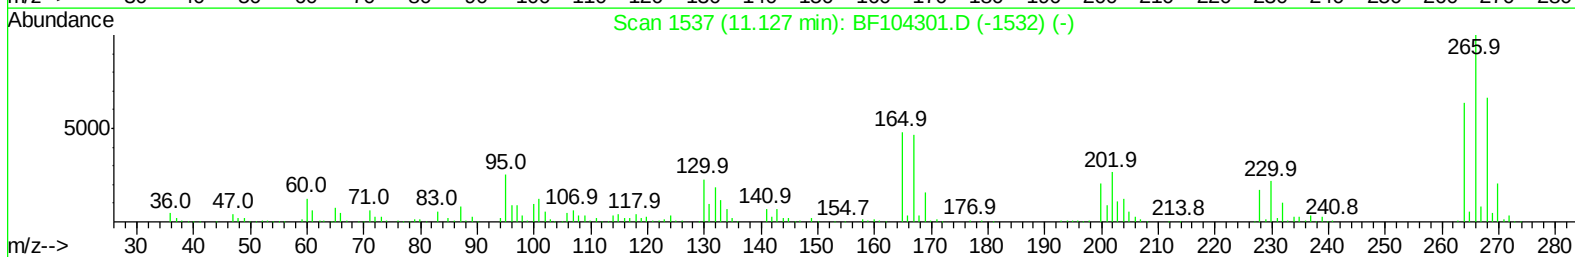
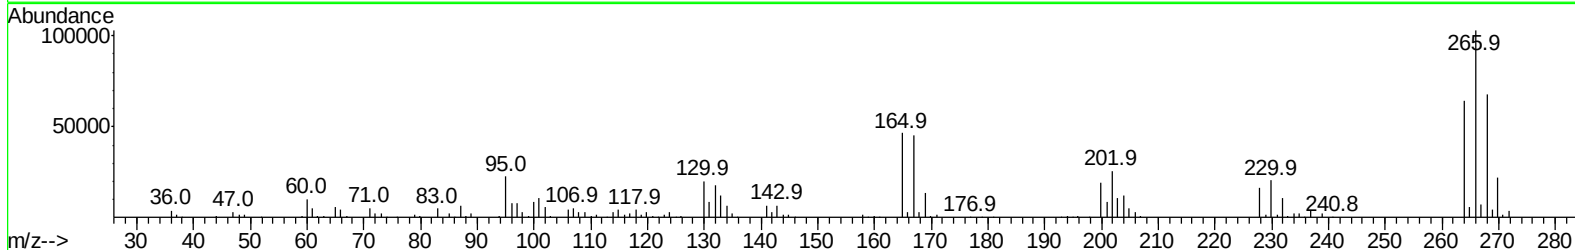


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041018\
Data File : BF104396.D
Acq On : 10 Apr 2018 8:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 02:13:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 12:04:31 2018
Response via : Initial Calibration

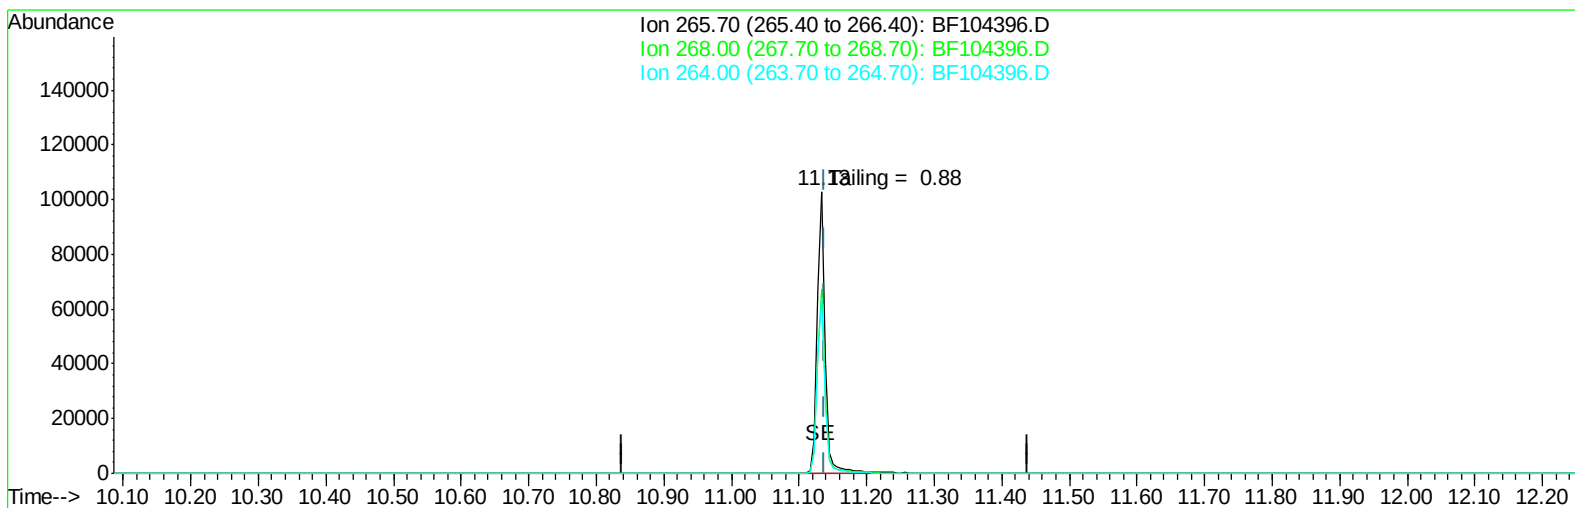

TIC: BF104396.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 38893.51ng

response 86971

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.61
264.00	61.90	62.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041018\
Data File : BF104396.D
Acq On : 10 Apr 2018 8:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 02:13:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 12:04:31 2018
Response via : Initial Calibration

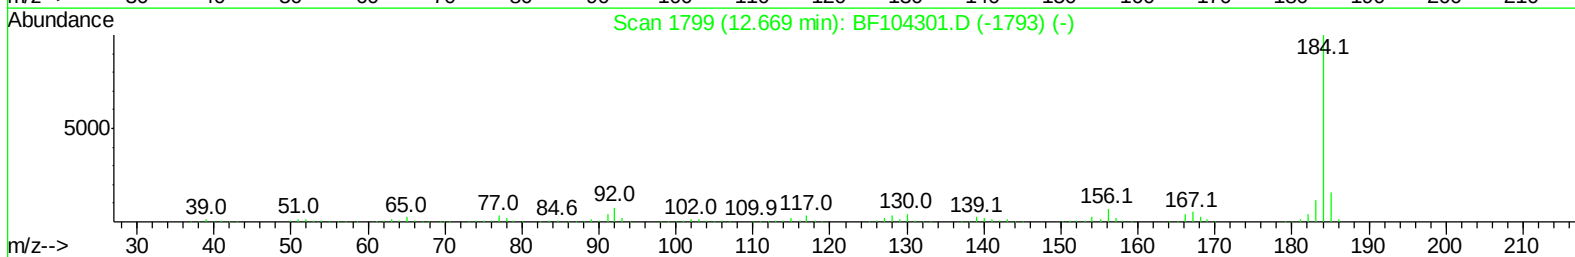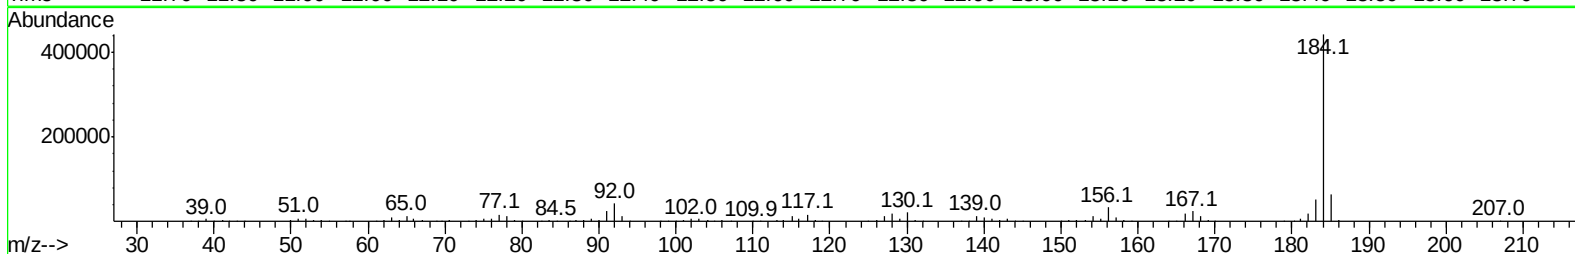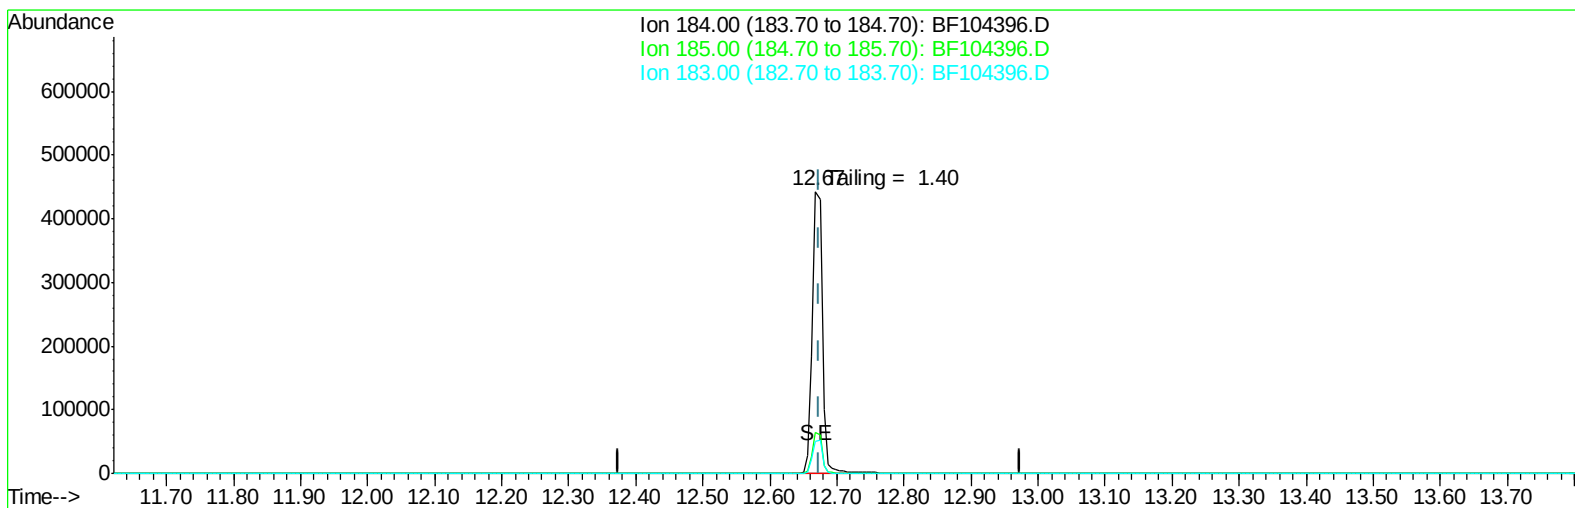

TIC: BF104396.D

(76) Benzidine

12.668min (-0.006) 0.00ng

response 438620

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.53
183.00	11.60	11.56
0.00	0.00	0.00