
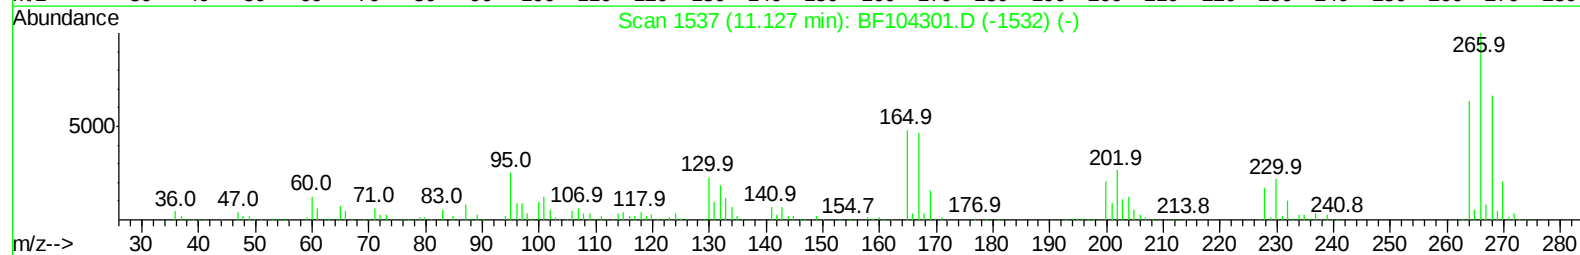
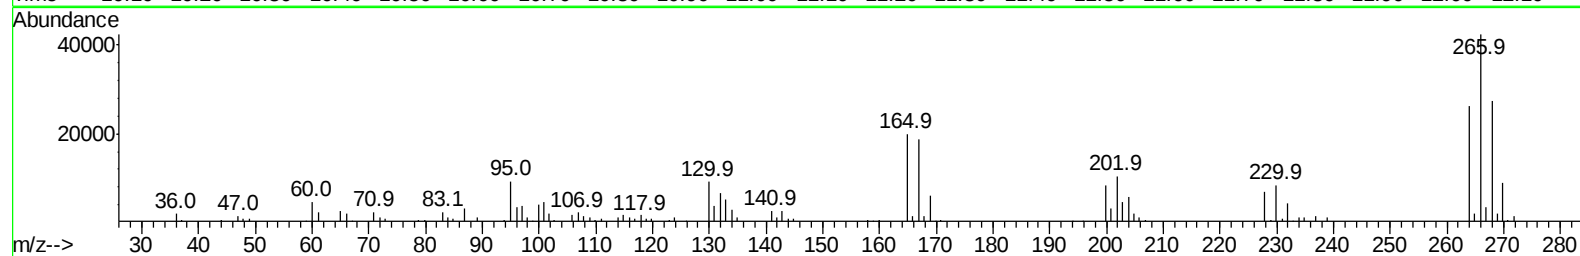


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041018\
Data File : BF104419.D
Acq On : 10 Apr 2018 20:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 02:15:46 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 12:04:31 2018
Response via : Initial Calibration

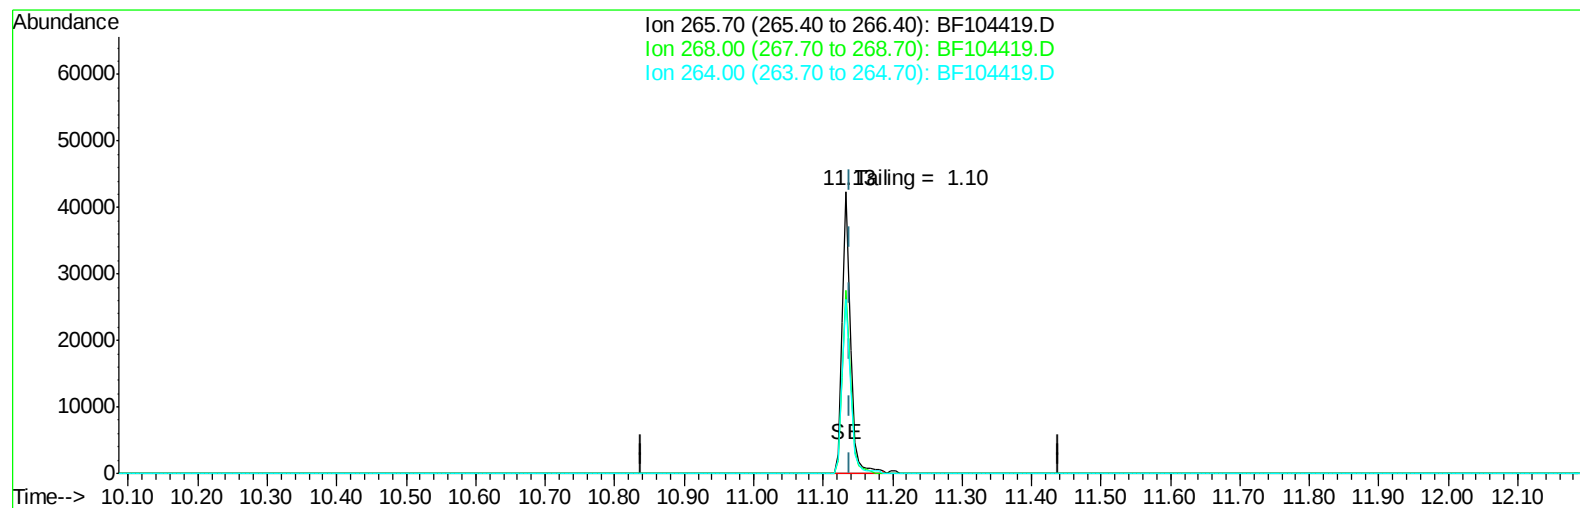

TIC: BF104419.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 0.00ng

response 34255

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.80
264.00	61.90	61.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041018\
Data File : BF104419.D
Acq On : 10 Apr 2018 20:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 02:15:46 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 12:04:31 2018
Response via : Initial Calibration

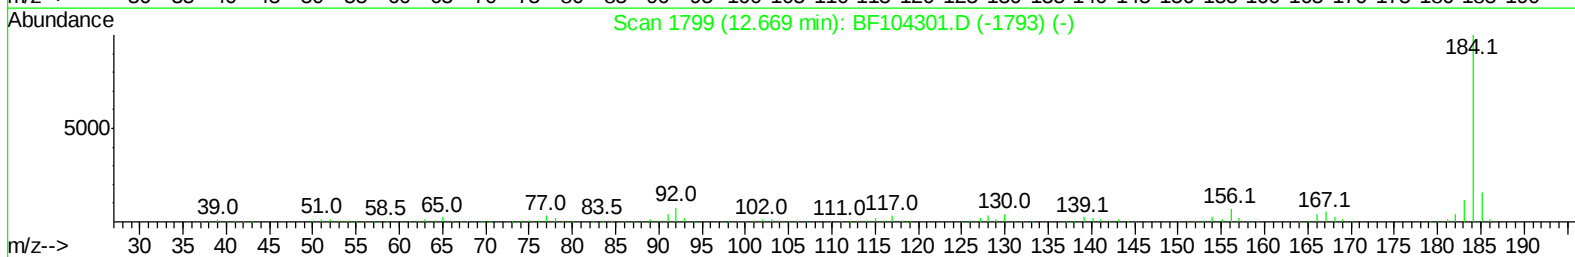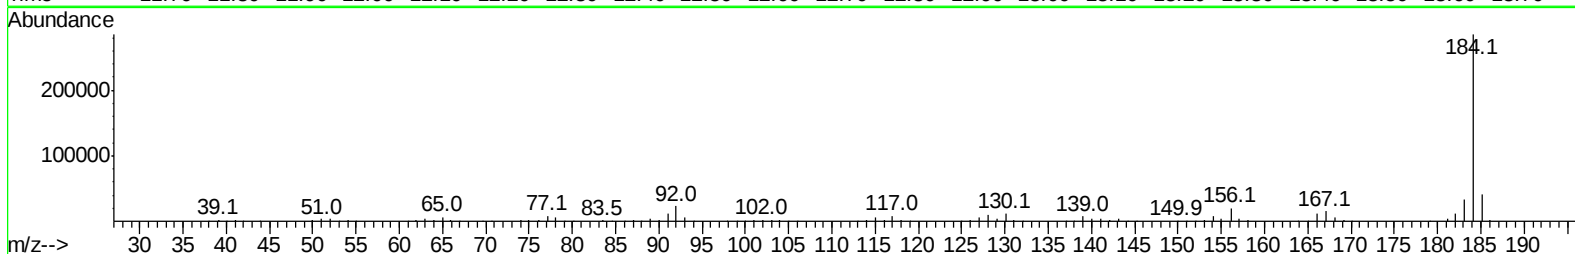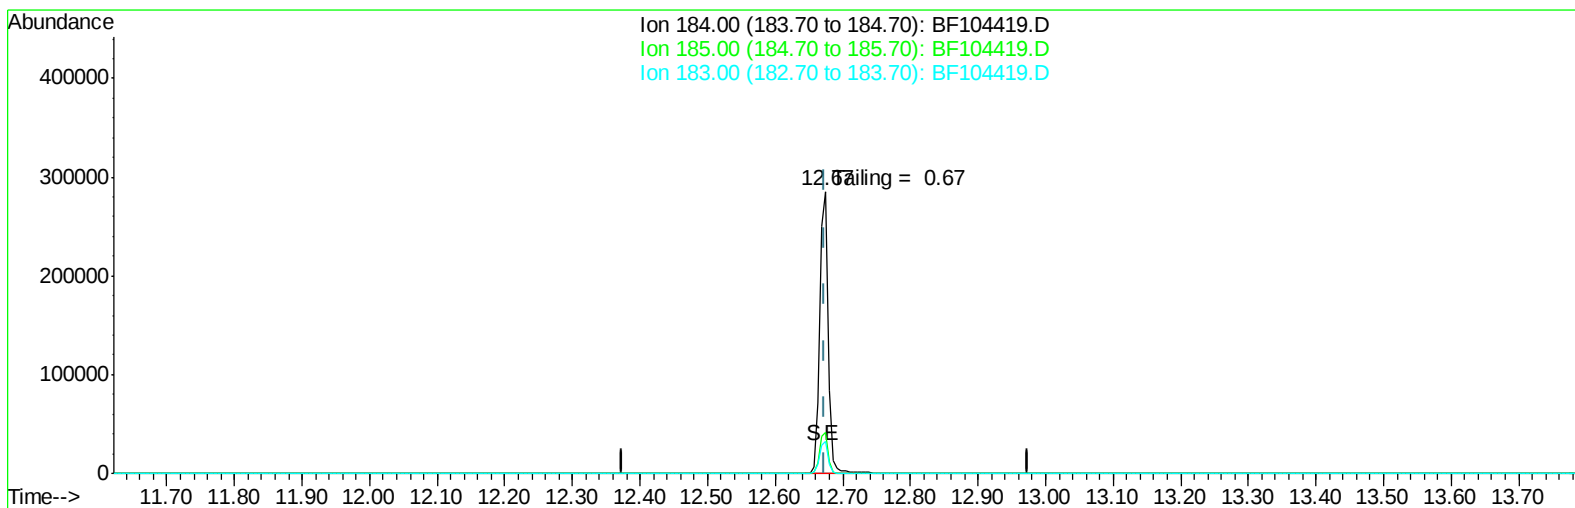

TIC: BF104419.D

(76) Benzidine

12.674min (+0.000) -20.00ng

response 258187

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.54
183.00	11.60	11.55
0.00	0.00	0.00