


Data Path : Z:\HPCHEM1\BNA F\Data\BF041018\
 Data File : BF104419.D
 Acq On : 10 Apr 2018 20:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 11 13:19:22 2018

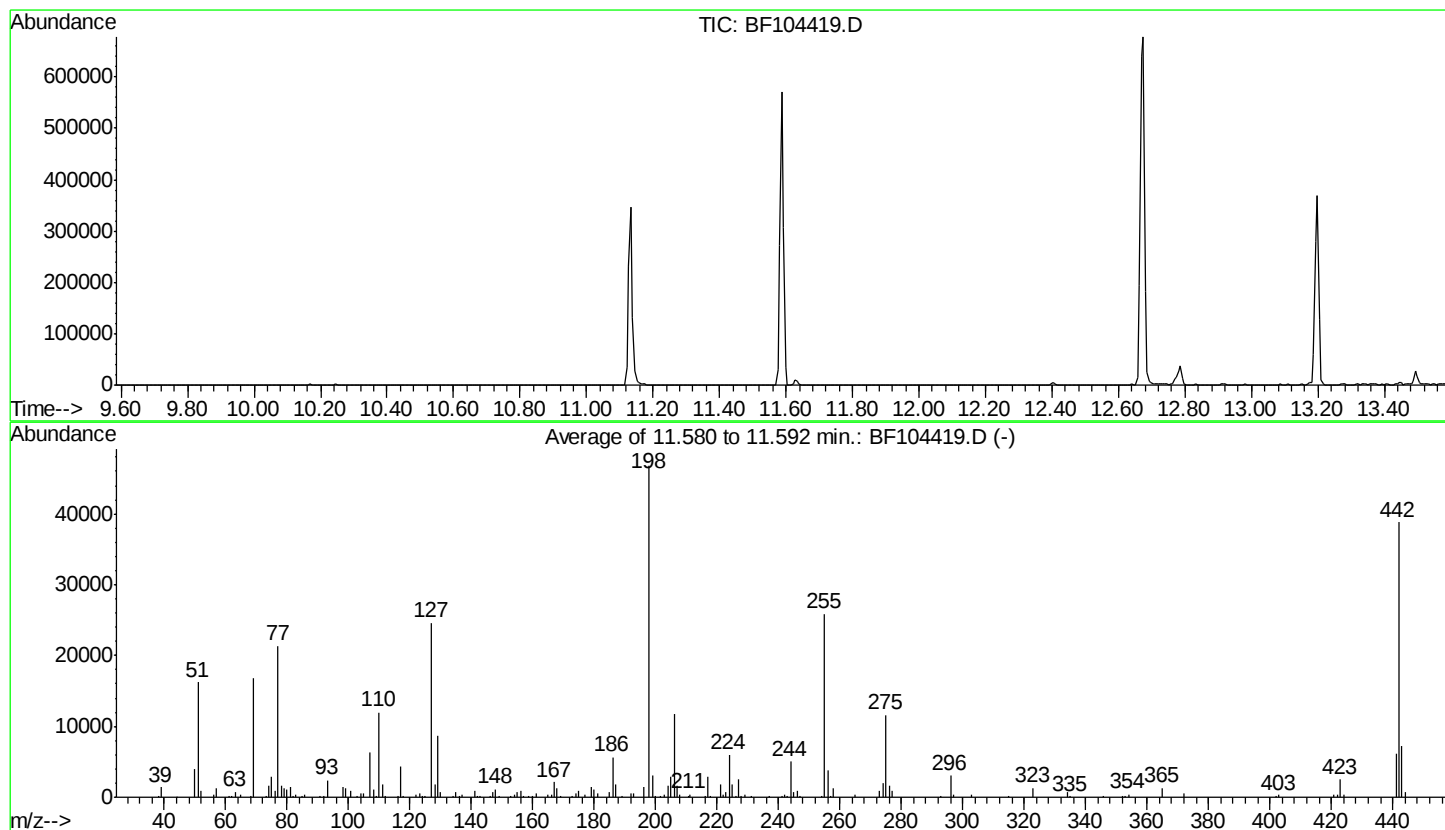

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	16194	PASS
68	69	0.00	2	0.8	128	PASS
69	198	0.00	100	35.8	16764	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	24604	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46810	PASS
199	198	5	9	6.4	2996	PASS
275	198	10	60	24.9	11640	PASS
365	198	1	100	2.9	1351	PASS
441	443	0.01	100	85.6	6159	PASS
442	198	50	100	83.0	38839	PASS
443	442	15	24	18.5	7194	PASS