
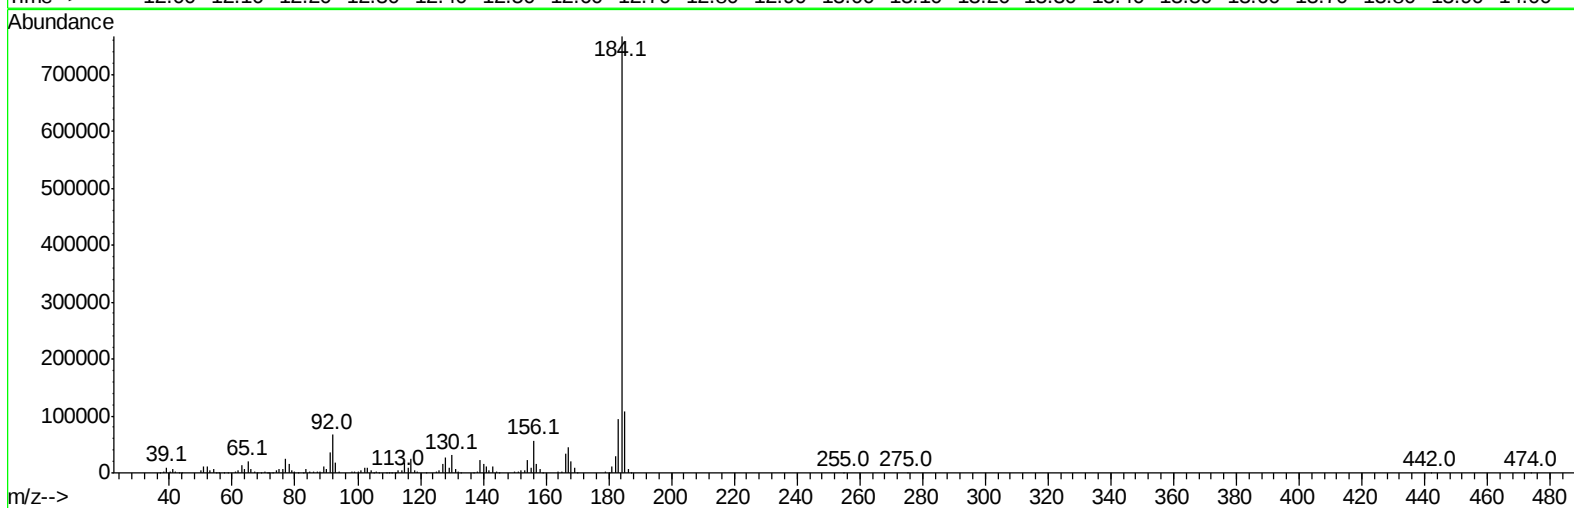


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041117\
 Data File : BF094352.D
 Acq On : 11 Apr 2017 15:31
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:00:12 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 13:20:29 2017
 Response via : Initial Calibration

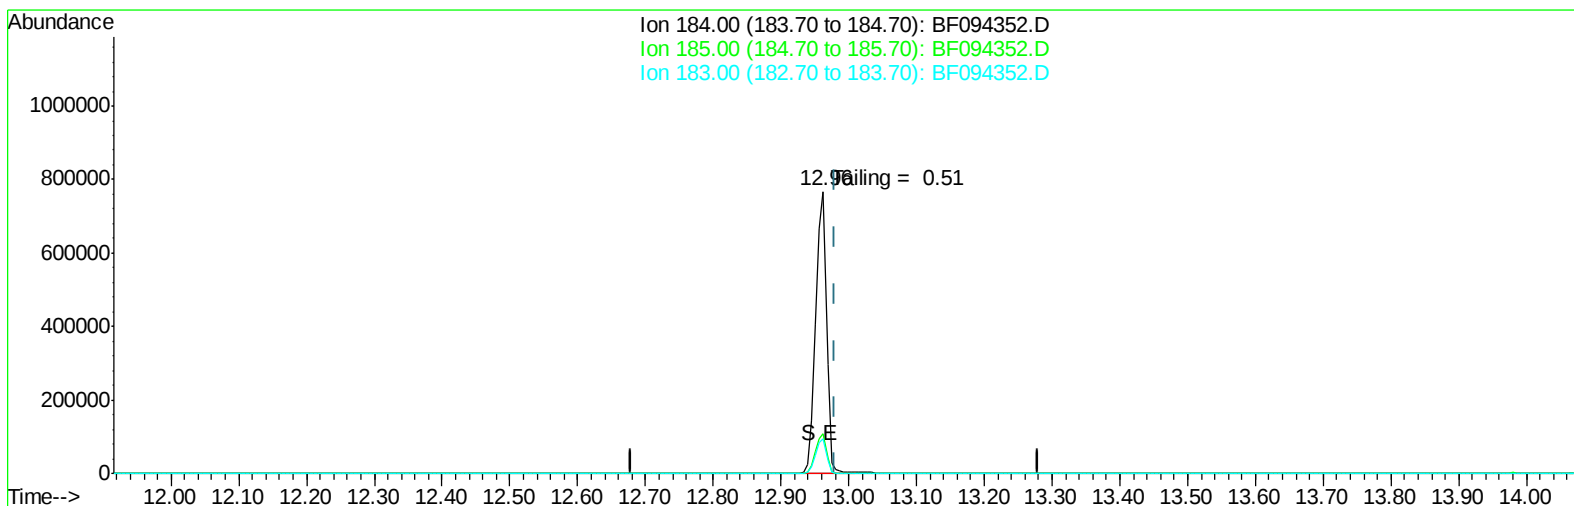

TIC: BF094352.D

(76) Benzidine



12.963min (-0.018) 0.00ng

response 841985

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.18#
183.00	12.20	12.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041117\
Data File : BF094352.D
Acq On : 11 Apr 2017 15:31
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:00:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

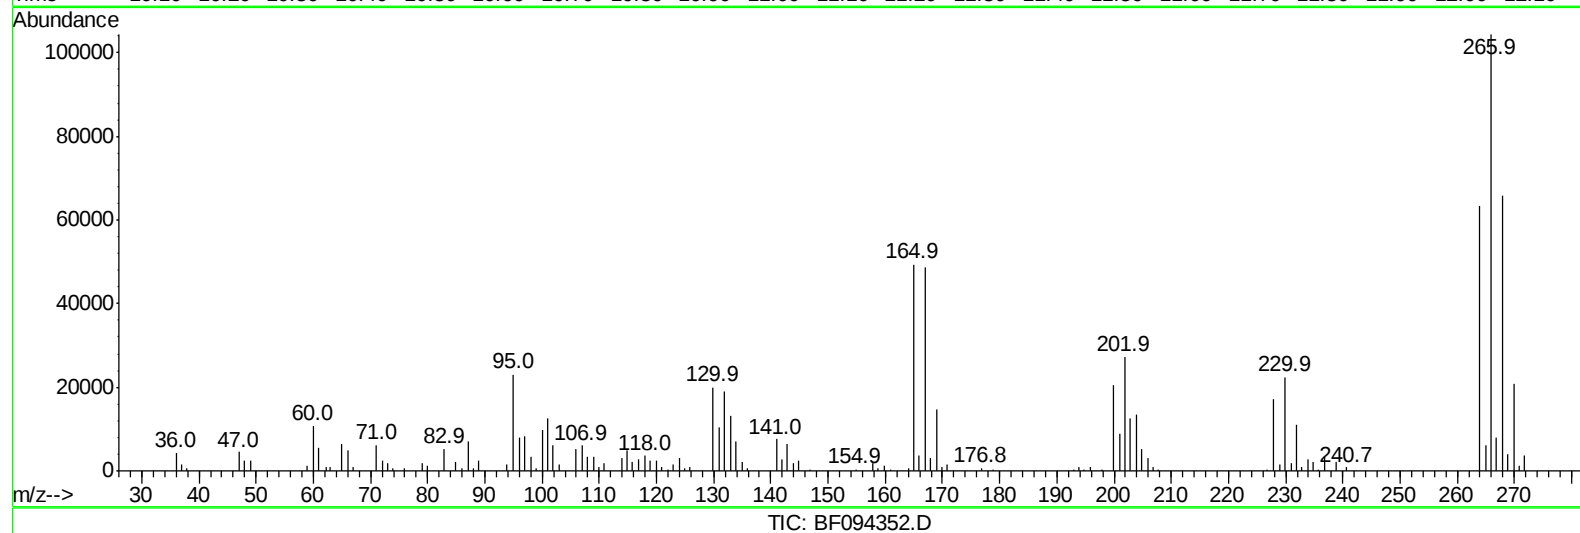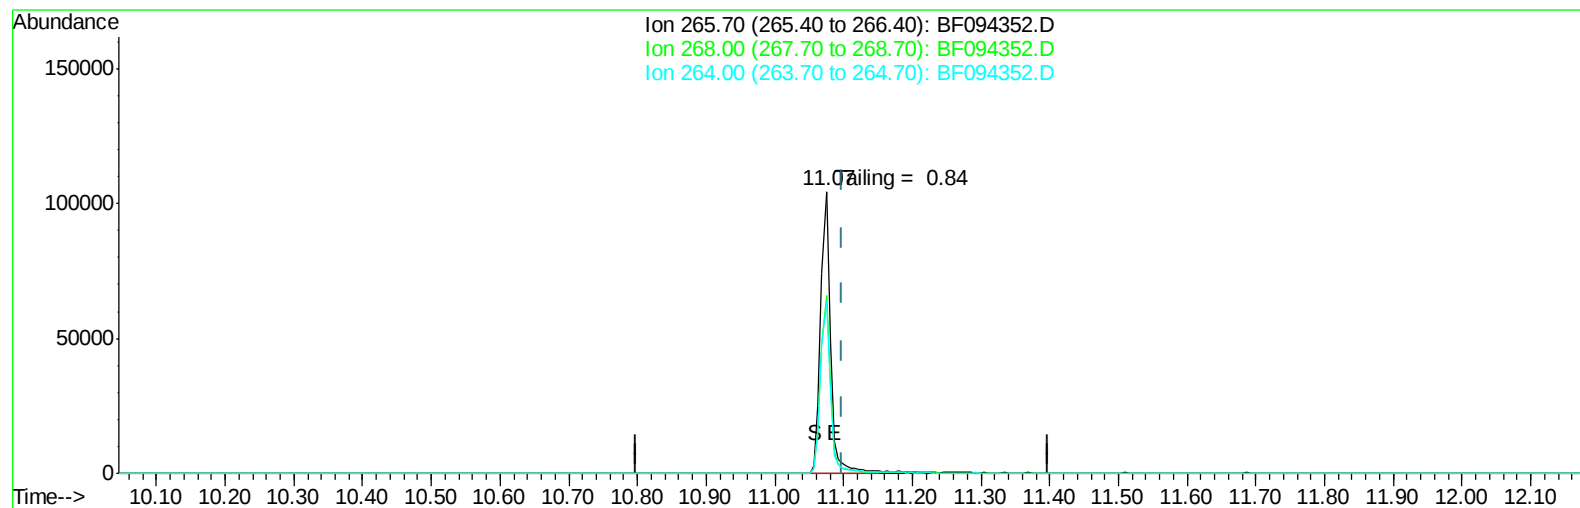

(69) Pentachlorophenol (C)

11.075min (-0.024) 0.00ng

response 102964

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.17
264.00	64.60	60.84
0.00	0.00	0.00