
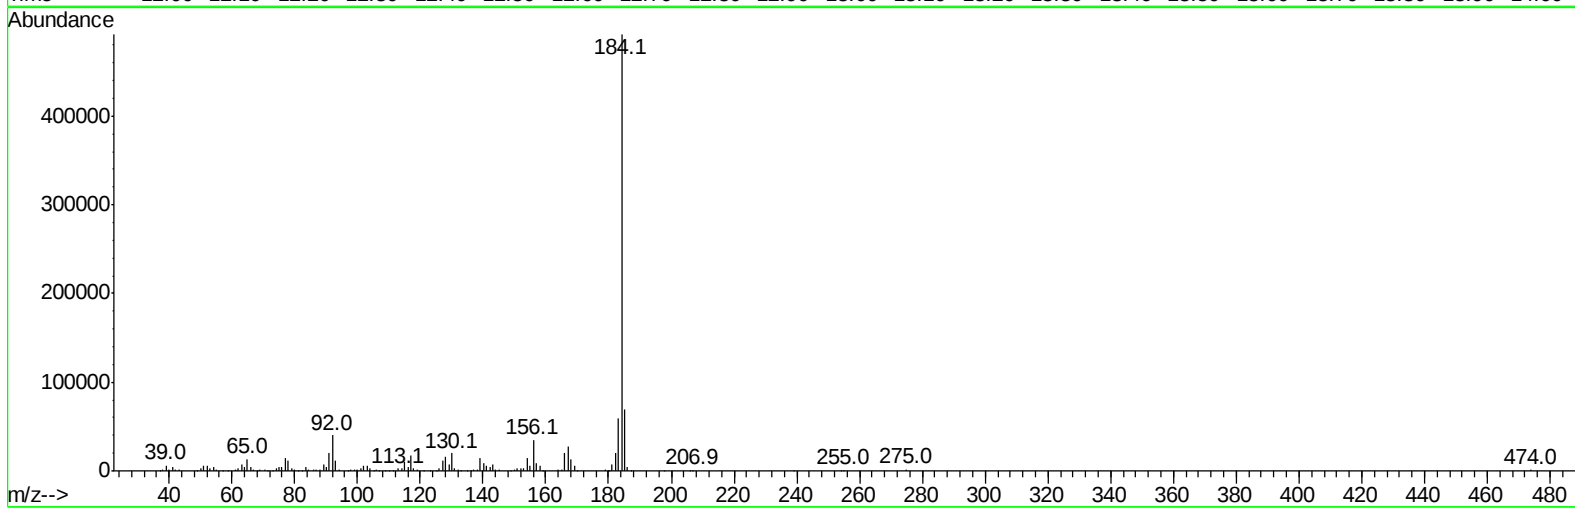


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041117\
Data File : BF094377.D
Acq On : 12 Apr 2017 5:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:08:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

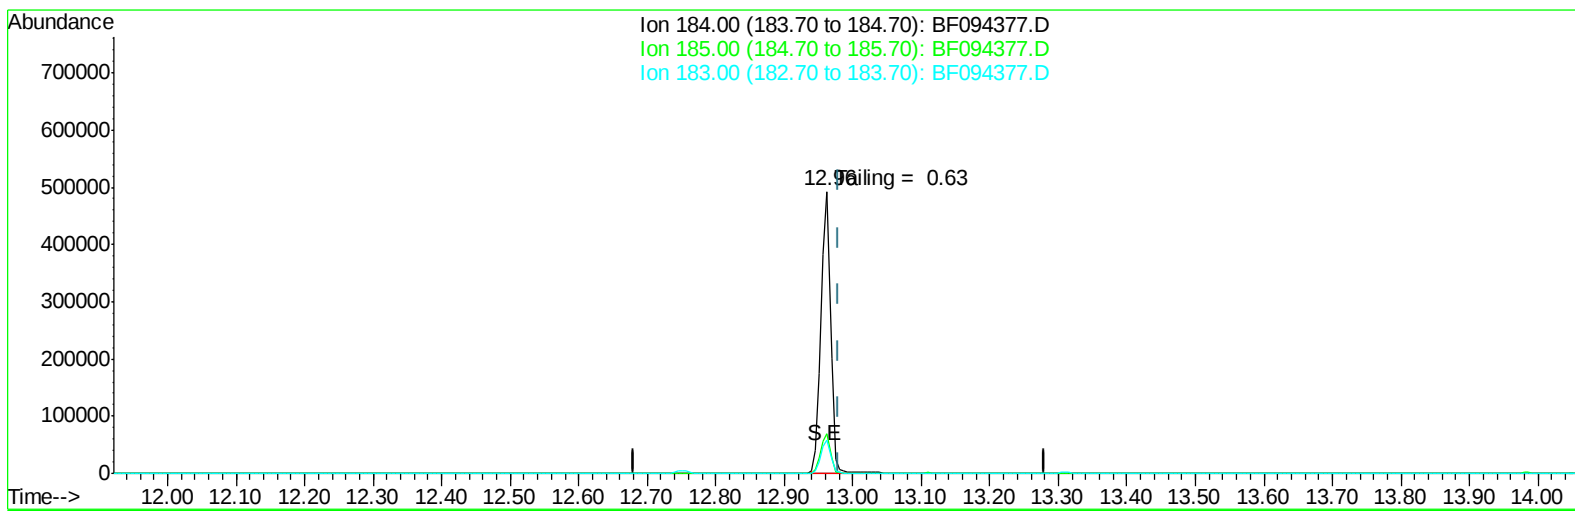

TIC: BF094377.D

(76) Benzidine



12.963min (-0.018) 15891.30ng

response 478002

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.97#
183.00	12.20	11.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041117\
Data File : BF094377.D
Acq On : 12 Apr 2017 5:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:08:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

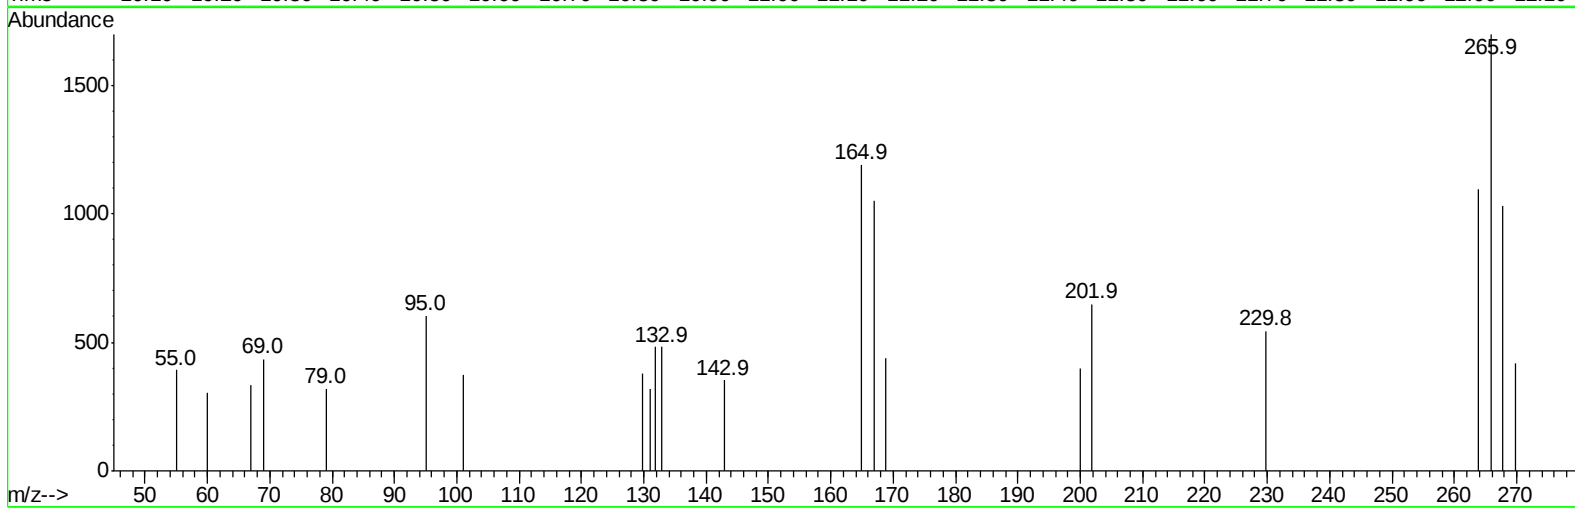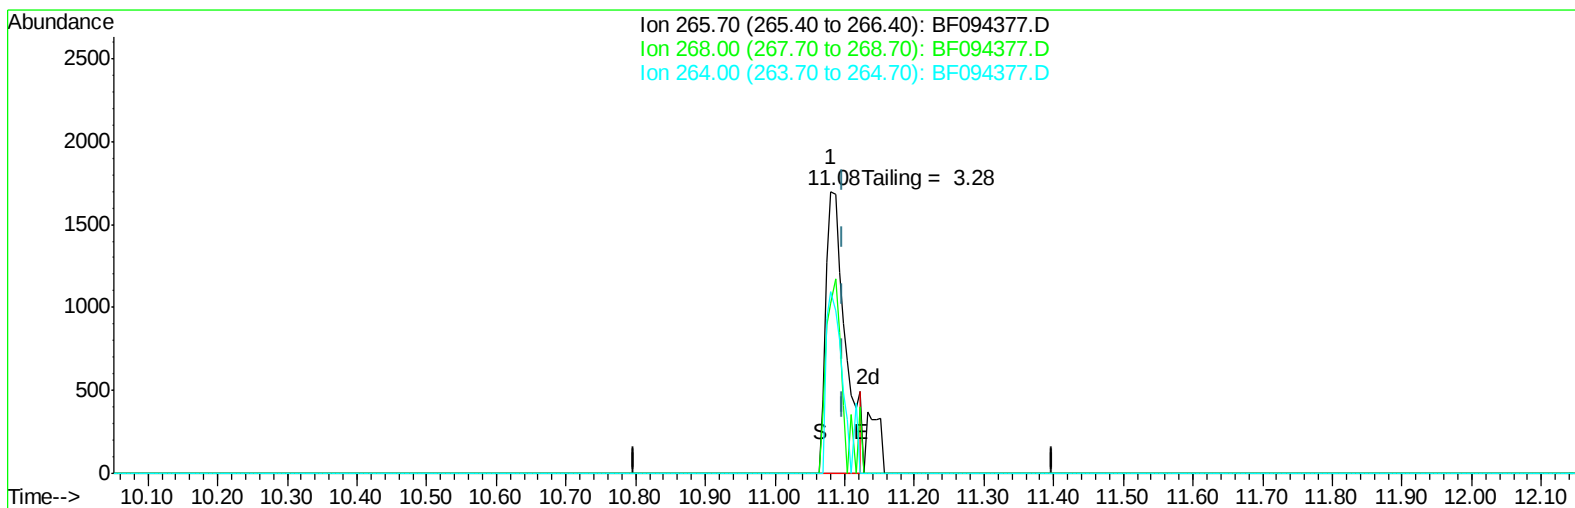

TIC: BF094377.D

(69) Pentachlorophenol (C)

11.080min (-0.018) 0.00ng m

response 3262

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.64
264.00	64.60	64.53
0.00	0.00	0.00