

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041117\
 Data File : BF094371.D
 Acq On : 12 Apr 2017 00:55
 Operator : SJ/MA
 Sample : I2622-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-AA8-BASE-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.322	407	414	420	rVV2	1350877	2079796	4.03%	0.417%
2	4.375	420	423	429	rVV	2182721	2429487	4.71%	0.487%
3	4.581	455	458	463	rVV2	928027	1049677	2.03%	0.210%
4	4.646	466	469	476	rVB	1309772	1361183	2.64%	0.273%
5	5.010	527	531	538	rVV2	1243794	1730951	3.35%	0.347%
6	5.310	579	582	586	rVV3	2137401	3018147	5.85%	0.605%
7	5.399	591	597	603	rBV2	3367190	7241183	14.03%	1.451%
8	5.498	606	614	618	rVV3	3906407	8607463	16.68%	1.725%
9	5.593	625	630	635	rVB	2089811	3195067	6.19%	0.640%
10	5.651	635	640	641	rBV	3795594	4744094	9.19%	0.951%
11	5.669	641	643	648	rVB	3705971	3553970	6.89%	0.712%
12	5.869	674	677	681	rVB2	1824834	1914906	3.71%	0.384%
13	5.910	681	684	689	rBV	1826007	2210688	4.28%	0.443%
14	5.993	694	698	699	rVV	975714	1395598	2.70%	0.280%
15	6.016	699	702	705	rVV2	2996970	4151366	8.04%	0.832%
16	6.046	705	707	712	rVB2	1255597	1555450	3.01%	0.312%
17	6.216	717	736	741	rBV4	7347531	33920070	65.72%	6.797%
18	6.310	747	752	755	rVB2	1162321	1908105	3.70%	0.382%
19	6.440	758	774	787	rBV7	7155515	51616195	100.00%	10.343%
20	6.534	787	790	792	rVB4	1113400	1164109	2.26%	0.233%
21	6.575	792	797	800	rVB	4586111	6001567	11.63%	1.203%
22	6.616	800	804	809	rVB4	1418548	2431367	4.71%	0.487%
23	6.698	809	818	824	rBV3	5082483	14185118	27.48%	2.842%
24	6.793	831	834	840	rVB4	2916585	4745602	9.19%	0.951%
25	6.922	840	856	862	rBV2	5003936	23562292	45.65%	4.721%
26	7.057	862	879	882	rBV8	4115329	19857676	38.47%	3.979%
27	7.251	891	912	917	rBV3	4866929	34673145	67.17%	6.948%
28	7.310	920	922	924	rVB	3841339	3451768	6.69%	0.692%
29	7.404	924	938	948	rBV7	5105293	24118683	46.73%	4.833%
30	7.487	948	952	955	rBV2	1804739	2698127	5.23%	0.541%
31	7.734	982	994	997	rBV	3945705	11585747	22.45%	2.321%
32	7.834	1007	1011	1012	rBV2	1591972	2047964	3.97%	0.410%
33	7.881	1013	1019	1022	rVB4	3548458	7459791	14.45%	1.495%
34	7.934	1023	1028	1030	rBV2	3040055	4801183	9.30%	0.962%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041117\
 Data File : BF094371.D
 Acq On : 12 Apr 2017 00:55
 Operator : SJ/MA
 Sample : I2622-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-AA8-BASE-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.157	1056	1066	1070	rBV2	4037421	10209567	19.78%	2.046%
36	8.351	1096	1099	1100	rBV	1189017	1383857	2.68%	0.277%
37	8.481	1118	1121	1122	rBV2	1065880	1234931	2.39%	0.247%
38	8.539	1128	1131	1134	rBV4	1223188	1433242	2.78%	0.287%
39	8.581	1135	1138	1142	rVB2	2072294	2621124	5.08%	0.525%
40	8.628	1143	1146	1148	rBV3	1510225	2032644	3.94%	0.407%
41	8.663	1149	1152	1159	rVB3	3325745	6032098	11.69%	1.209%
42	8.810	1173	1177	1178	rBV3	1378611	1841926	3.57%	0.369%
43	9.028	1208	1214	1218	rVB	2796375	6198618	12.01%	1.242%
44	9.128	1223	1231	1233	rBV2	2677475	6748428	13.07%	1.352%
45	9.345	1265	1268	1271	rVB	2057983	2249988	4.36%	0.451%
46	9.504	1288	1295	1298	rBV2	3795963	7541544	14.61%	1.511%
47	9.657	1316	1321	1326	rVV3	2308030	4638263	8.99%	0.929%
48	9.704	1326	1329	1332	rVB2	1589375	1741128	3.37%	0.349%
49	9.781	1335	1342	1344	rVV5	2586921	5756469	11.15%	1.153%
50	9.810	1344	1347	1348	rVV	1791049	2074772	4.02%	0.416%
51	9.834	1349	1351	1354	rVV2	2736970	2940539	5.70%	0.589%
52	9.881	1356	1359	1362	rVV3	2420956	2930523	5.68%	0.587%
53	9.922	1362	1366	1368	rVV2	2737422	3585506	6.95%	0.718%
54	9.951	1368	1371	1374	rVB	2348578	2718831	5.27%	0.545%
55	10.116	1393	1399	1402	rBV2	3368657	5656078	10.96%	1.133%
56	10.181	1407	1410	1414	rVB	2119526	2414915	4.68%	0.484%
57	10.233	1414	1419	1421	rBV2	1706708	2940529	5.70%	0.589%
58	10.339	1435	1437	1439	rBV3	846992	1040101	2.02%	0.208%
59	10.375	1440	1443	1447	rVB2	2303344	3121883	6.05%	0.626%
60	10.469	1457	1459	1461	rBV2	1073502	1174188	2.27%	0.235%
61	10.492	1461	1463	1468	rVV4	1638123	2156834	4.18%	0.432%
62	10.651	1487	1490	1492	rBV	1207381	1261123	2.44%	0.253%
63	10.698	1492	1498	1500	rBV	3388233	7142697	13.84%	1.431%
64	10.898	1529	1532	1534	rBV	1040588	1181756	2.29%	0.237%
65	11.033	1552	1555	1560	rVV4	1218440	2070558	4.01%	0.415%
66	11.081	1560	1563	1566	rVB2	1171526	1281910	2.48%	0.257%
67	11.245	1585	1591	1593	rBV	3454571	5592351	10.83%	1.121%
68	11.280	1593	1597	1600	rVB	3113193	3913783	7.58%	0.784%
69	11.775	1676	1681	1684	rVB	3420118	4775946	9.25%	0.957%
70	11.957	1707	1712	1714	rBV3	1412953	2229686	4.32%	0.447%
71	11.992	1714	1718	1722	rVB2	2133978	2977790	5.77%	0.597%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041117\
 Data File : BF094371.D
 Acq On : 12 Apr 2017 00:55
 Operator : SJ/MA
 Sample : I2622-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-AA8-BASE-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.039	1723	1726	1729	rBV2	1652398	1928506	3.74%	0.386%
73	12.086	1730	1734	1736	rBV2	1511200	2496810	4.84%	0.500%
74	12.163	1745	1747	1751	rVB2	1197771	1354989	2.63%	0.272%
75	12.275	1762	1766	1769	rVB	2955867	3515666	6.81%	0.704%
76	12.310	1769	1772	1775	rBV2	1520614	1659433	3.21%	0.333%
77	12.339	1775	1777	1784	rVB3	1347188	2109616	4.09%	0.423%
78	12.416	1785	1790	1792	rBV	2231995	3019179	5.85%	0.605%
79	12.463	1792	1798	1804	rBV3	1475354	3102053	6.01%	0.622%
80	12.639	1825	1828	1831	rVB4	1210734	1386476	2.69%	0.278%
81	12.675	1831	1834	1839	rVB3	1839613	2373618	4.60%	0.476%
82	12.751	1841	1847	1849	rVB2	2628231	4287556	8.31%	0.859%
83	12.798	1849	1855	1859	rBV4	1902803	3635122	7.04%	0.728%
84	12.845	1860	1863	1866	rVB	1330414	1424388	2.76%	0.285%
85	13.210	1922	1925	1931	rVB	2298256	3207802	6.21%	0.643%
86	13.286	1935	1938	1940	rVB2	1400833	1471106	2.85%	0.295%
87	13.363	1946	1951	1961	rVB4	2047003	4700200	9.11%	0.942%
88	13.486	1965	1972	1975	rVV	3039727	5305855	10.28%	1.063%
89	13.557	1979	1984	1991	rVB4	2430650	3569365	6.92%	0.715%
90	13.645	1996	1999	2002	rVV	1805106	2262229	4.38%	0.453%
91	13.692	2004	2007	2015	rVB5	1582209	2670533	5.17%	0.535%
92	13.839	2028	2032	2036	rVV	1344643	1578041	3.06%	0.316%
93	13.916	2040	2045	2047	rVV	2401252	3410690	6.61%	0.683%
94	13.939	2047	2049	2058	rVB	751804	1151654	2.23%	0.231%
95	14.063	2068	2070	2074	rVB	1254772	1282577	2.48%	0.257%
96	14.292	2106	2109	2113	rBV3	673674	1273815	2.47%	0.255%
97	16.339	2453	2457	2462	rVB2	842627	1060594	2.05%	0.213%
98	16.910	2549	2554	2570	rVB2	2244272	4203686	8.14%	0.842%
99	18.680	2850	2855	2866	rVB3	457014	1087761	2.11%	0.218%
100	18.956	2897	2902	2914	rVB2	487299	1224084	2.37%	0.245%


Sum of corrected areas: 499067065

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041117\
Data File : BF094371.D
Acq On : 12 Apr 2017 00:55
Operator : SJ/MA
Sample : I2622-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-AA8-BASE-D

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

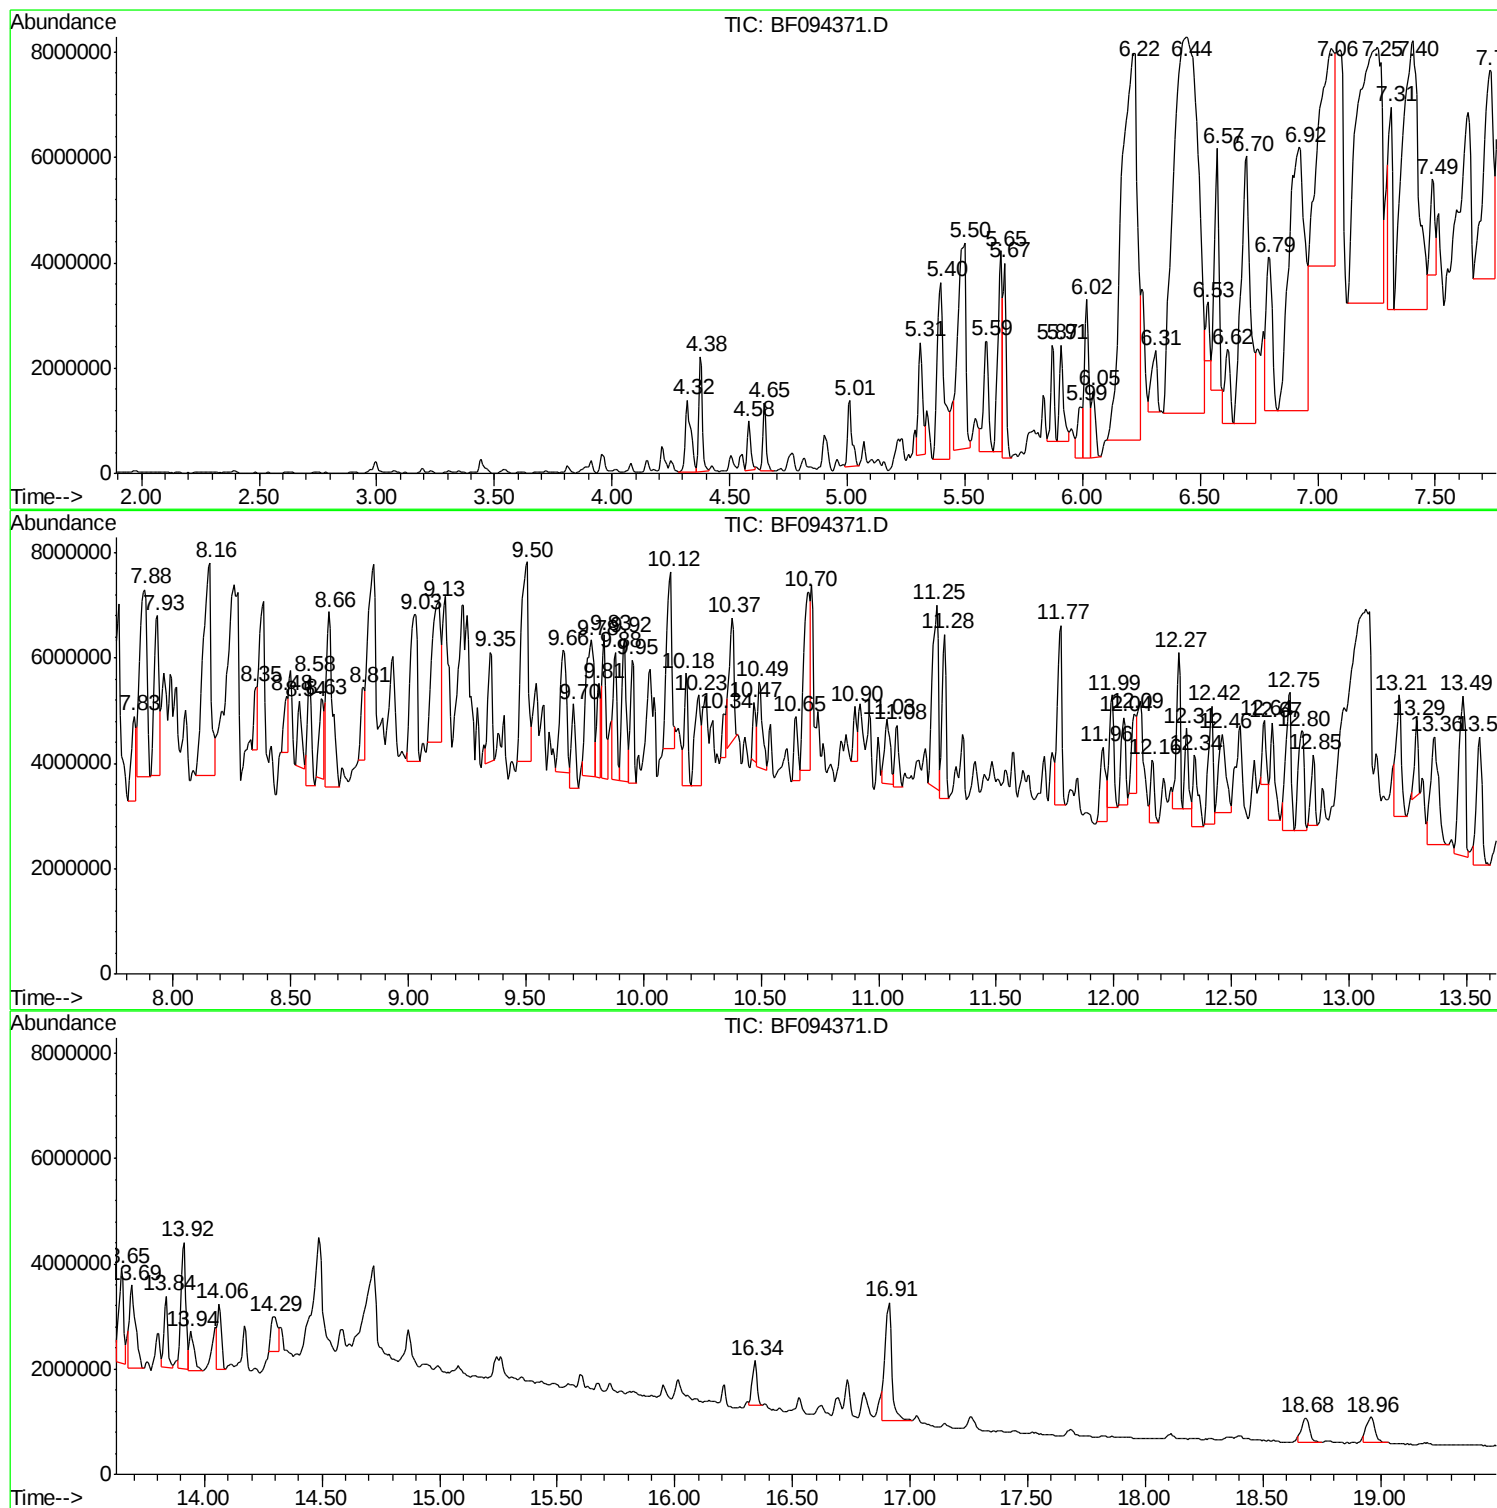

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF041117\
Data_File : BF094371.D
Acq_On : 12-Apr-2017 00:555
Operator : SJ/MAA
Sample : I2622-088
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-AA8-BASE-D

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
