


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041117\
 Data File : BF094352.D
 Acq On : 11 Apr 2017 15:31
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 13:20:29 2017

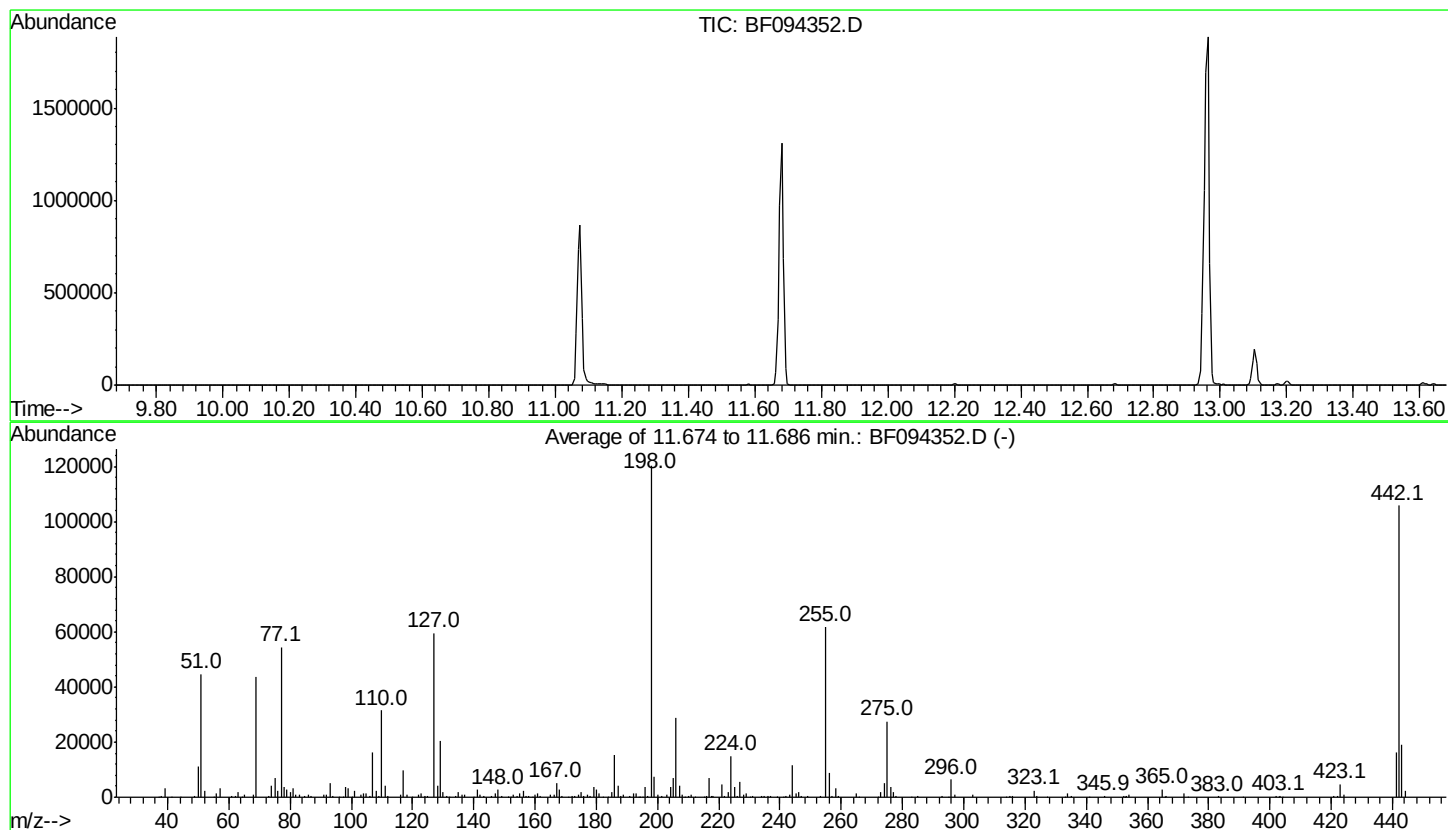

AutoFind: Scans 1664, 1665, 1666; Background Corrected with Scan 1657

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	44602	PASS
68	69	0.00	2	1.7	730	PASS
69	198	0.00	100	36.5	43856	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	59461	PASS
197	198	0.00	2	0.5	590	PASS
198	198	100	100	100.0	120269	PASS
199	198	5	9	6.3	7549	PASS
275	198	10	60	22.8	27474	PASS
365	198	1	100	2.4	2845	PASS
441	442	0.01	24	15.4	16238	PASS
442	198	50	100	87.8	105653	PASS
443	442	15	24	18.0	19023	PASS