


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041117\
 Data File : BF094377.D
 Acq On : 12 Apr 2017 5:04
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 13:20:29 2017

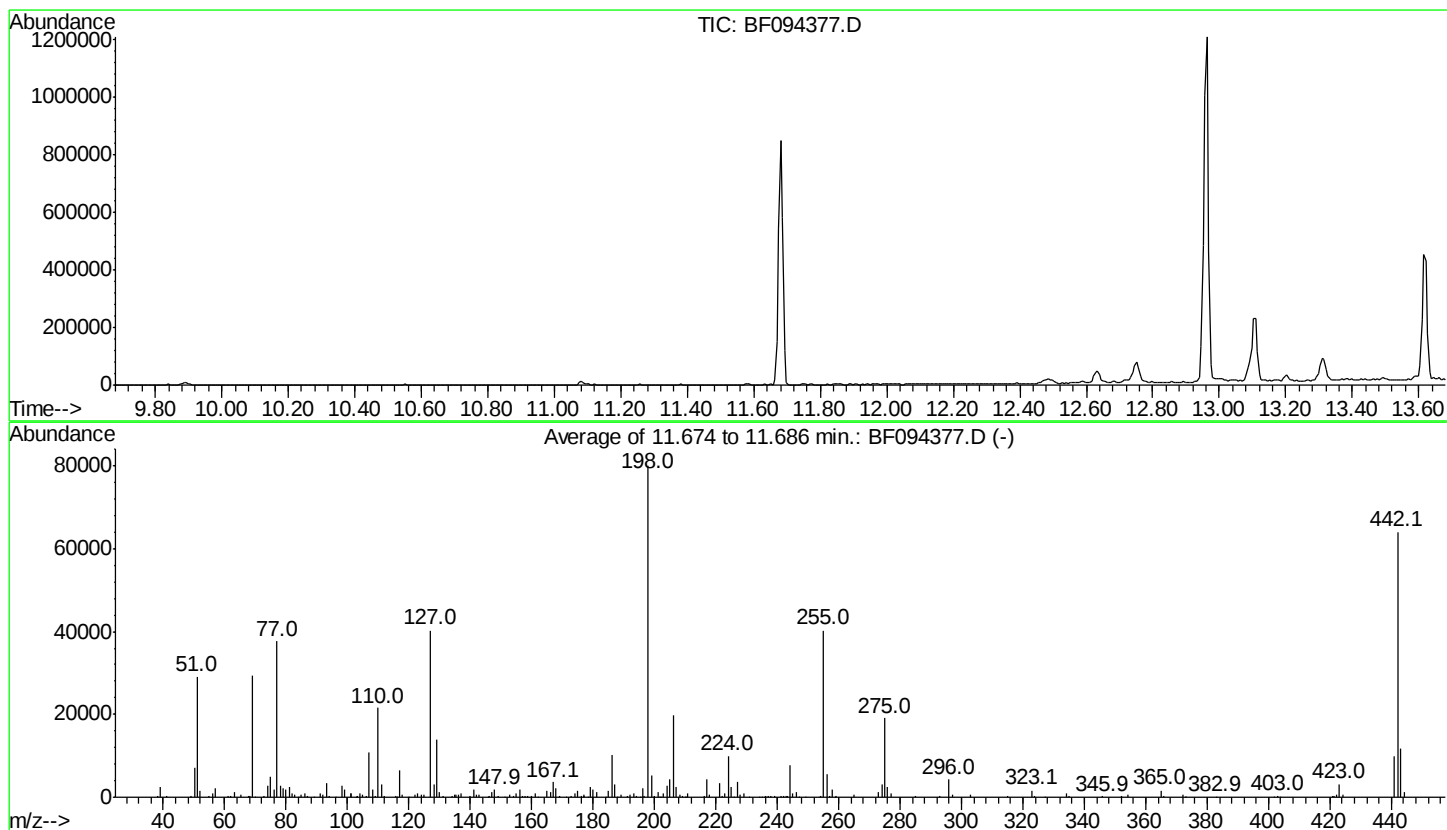

AutoFind: Scans 1664, 1665, 1666; Background Corrected with Scan 1659

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	29117	PASS
68	69	0.00	2	0.9	254	PASS
69	198	0.00	100	36.8	29424	PASS
70	69	0.00	2	0.4	116	PASS
127	198	10	80	50.3	40298	PASS
197	198	0.00	2	0.3	273	PASS
198	198	100	100	100.0	80048	PASS
199	198	5	9	6.4	5152	PASS
275	198	10	60	23.8	19025	PASS
365	198	1	100	2.1	1681	PASS
441	442	0.01	24	15.5	9906	PASS
442	198	50	100	80.0	64072	PASS
443	442	15	24	18.5	11841	PASS