


Data Path : Z:\HPCHEM1\BNA F\Data\BF041118\
 Data File : BF104424.D
 Acq On : 11 Apr 2018 8:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 11 13:19:22 2018

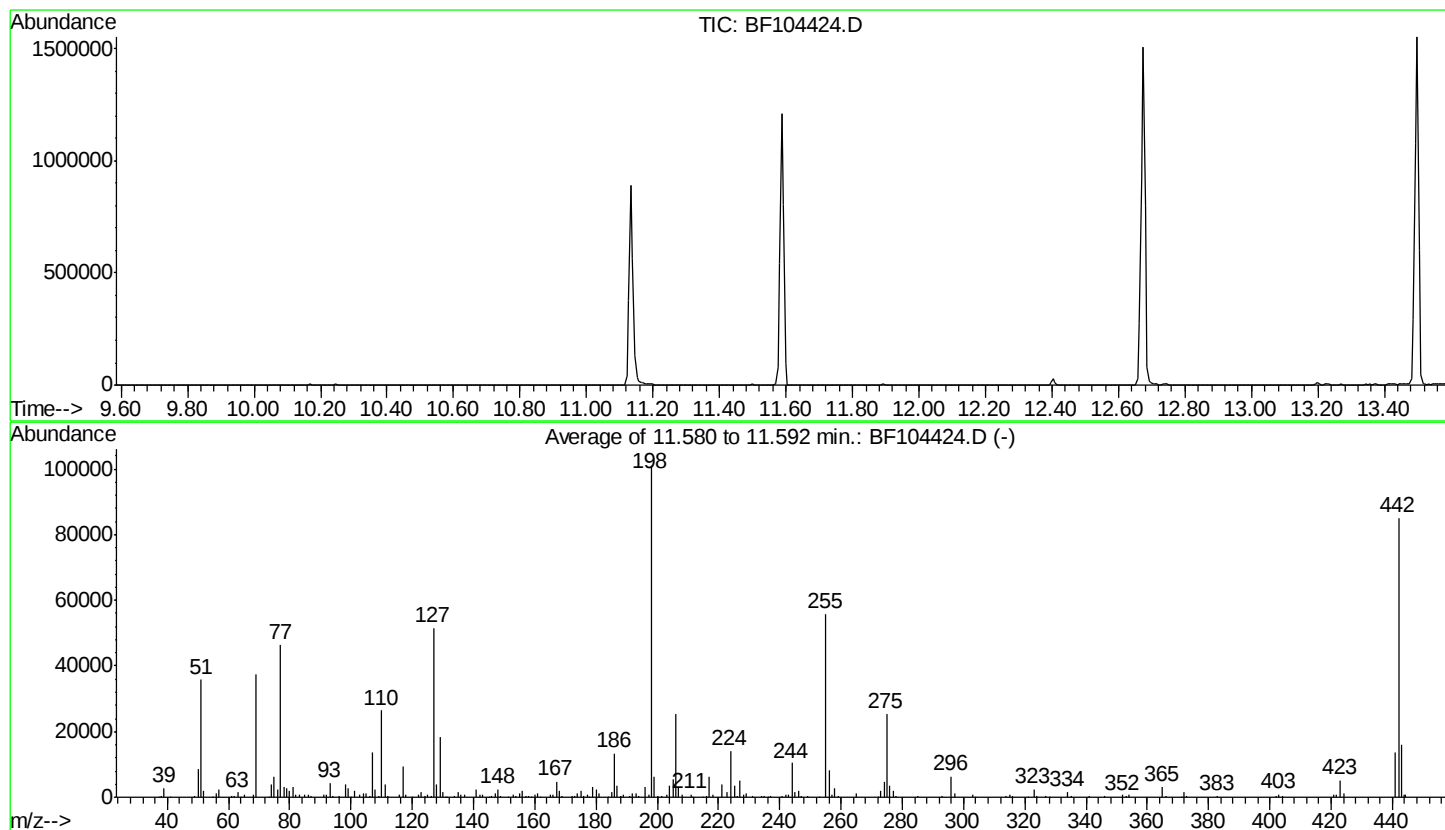

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	35714	PASS
68	69	0.00	2	1.7	651	PASS
69	198	0.00	100	36.9	37338	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	51576	PASS
197	198	0.00	2	0.6	635	PASS
198	198	100	100	100.0	101056	PASS
199	198	5	9	6.3	6409	PASS
275	198	10	60	25.1	25415	PASS
365	198	1	100	3.1	3136	PASS
441	443	0.01	100	84.0	13575	PASS
442	198	50	100	84.2	85090	PASS
443	442	15	24	19.0	16164	PASS