
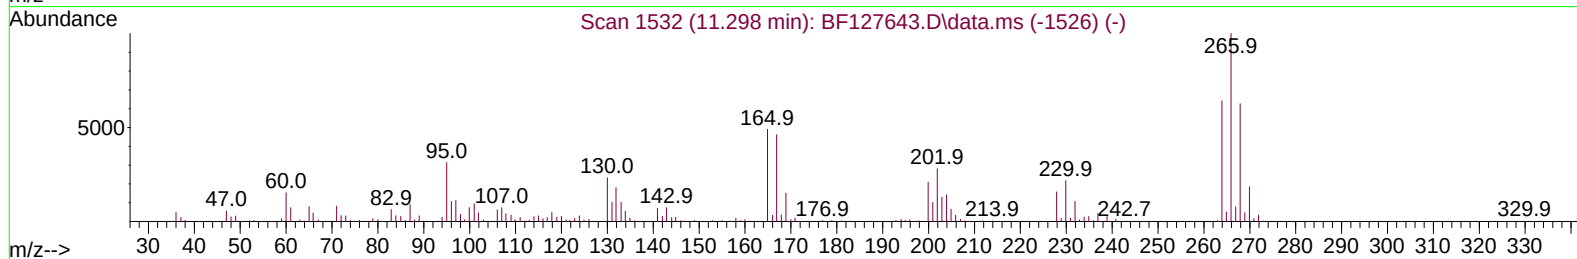
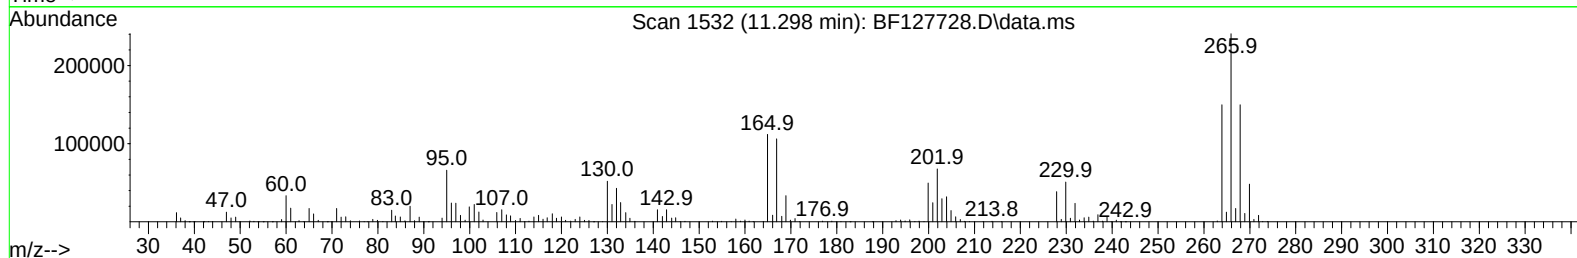


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
 Data File : BF127728.D
 Acq On : 11 Apr 2022 09:32
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 18:58:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 06 13:55:27 2022
 Response via : Initial Calibration

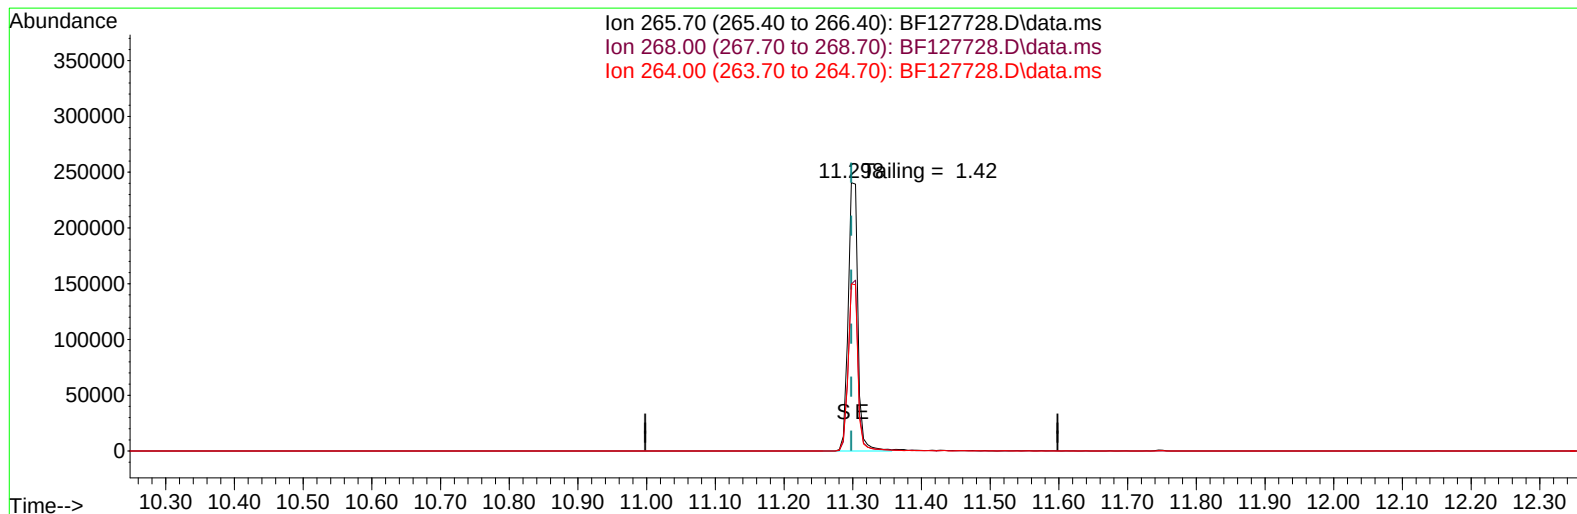

TIC: BF127728.D\data.ms

(70) Pentachlorophenol (C)




11.298min (-0.000) 393219.19 ng

response 236797

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.21
264.00	60.60	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127728.D
Acq On : 11 Apr 2022 09:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 18:58:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:55:27 2022
Response via : Initial Calibration

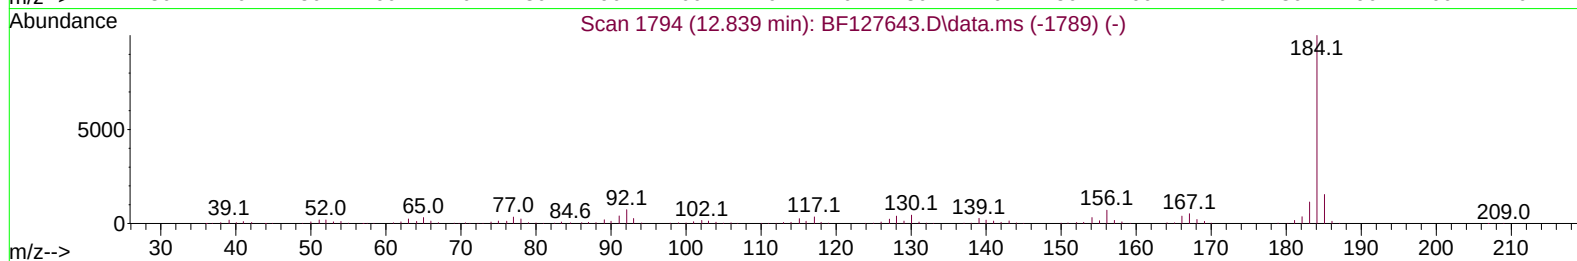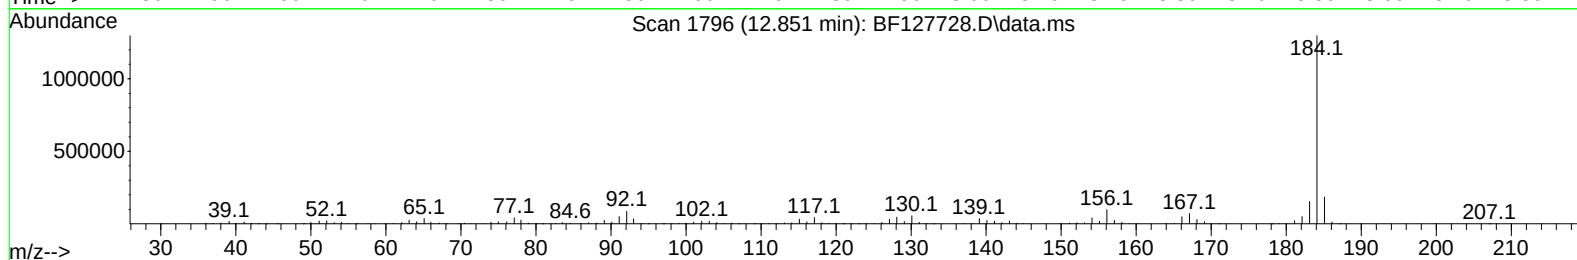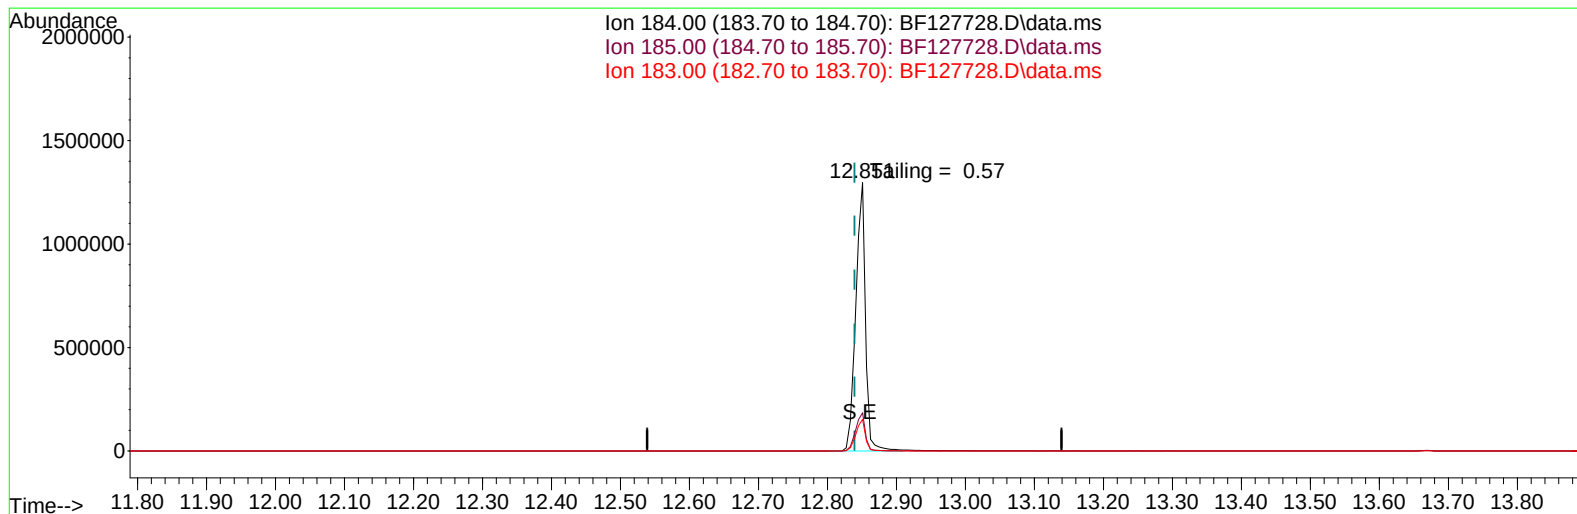

TIC: BF127728.D\data.ms

(77) Benzidine

12.851min (+ 0.012) 5973.84 ng m

response 1257194

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.25
183.00	11.70	11.81
0.00	0.00	0.00