

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
 Data File : BF127737.D
 Acq On : 11 Apr 2022 14:30
 Operator : CG\JU
 Sample : N2335-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A350-CU

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	138	144	151	rVB	281050	400365	7.04%	1.243%
2	4.810	425	429	435	rVB	473067	469457	8.26%	1.457%
3	5.234	496	501	509	rVB	465754	503885	8.87%	1.564%
4	5.604	558	564	567	rBV	3597010	3819075	67.20%	11.854%
5	6.592	726	732	735	rBV	3230612	3632978	63.92%	11.276%
6	6.963	792	795	801	rVB	964914	817814	14.39%	2.538%
7	7.534	886	892	894	rBV	2567938	2850773	50.16%	8.848%
8	8.245	1009	1013	1017	rBV	1120825	1038088	18.26%	3.222%
9	9.328	1191	1197	1200	rBV	5301616	5103425	89.79%	15.840%
10	10.010	1308	1313	1316	rBV	1460702	1241301	21.84%	3.853%
11	10.804	1443	1448	1451	rBV	3635018	3520638	61.94%	10.927%
12	11.504	1563	1567	1570	rBV	1498487	1318115	23.19%	4.091%
13	13.098	1832	1838	1841	rBV	5693903	5683568	100.00%	17.641%
14	14.151	2013	2017	2024	rVB	1177014	1001126	17.61%	3.107%
15	15.680	2271	2277	2285	rBV	593084	817646	14.39%	2.538%




Sum of corrected areas: 32218254

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127737.D
Acq On : 11 Apr 2022 14:30
Operator : CG\JU
Sample : N2335-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A350-CU

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

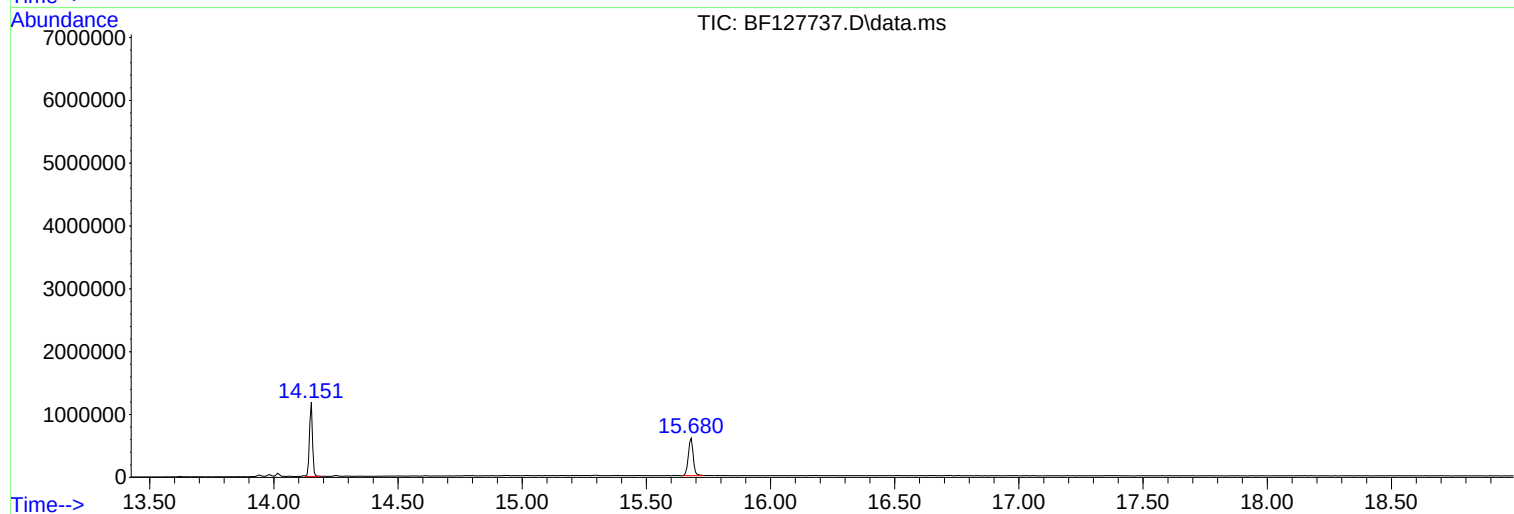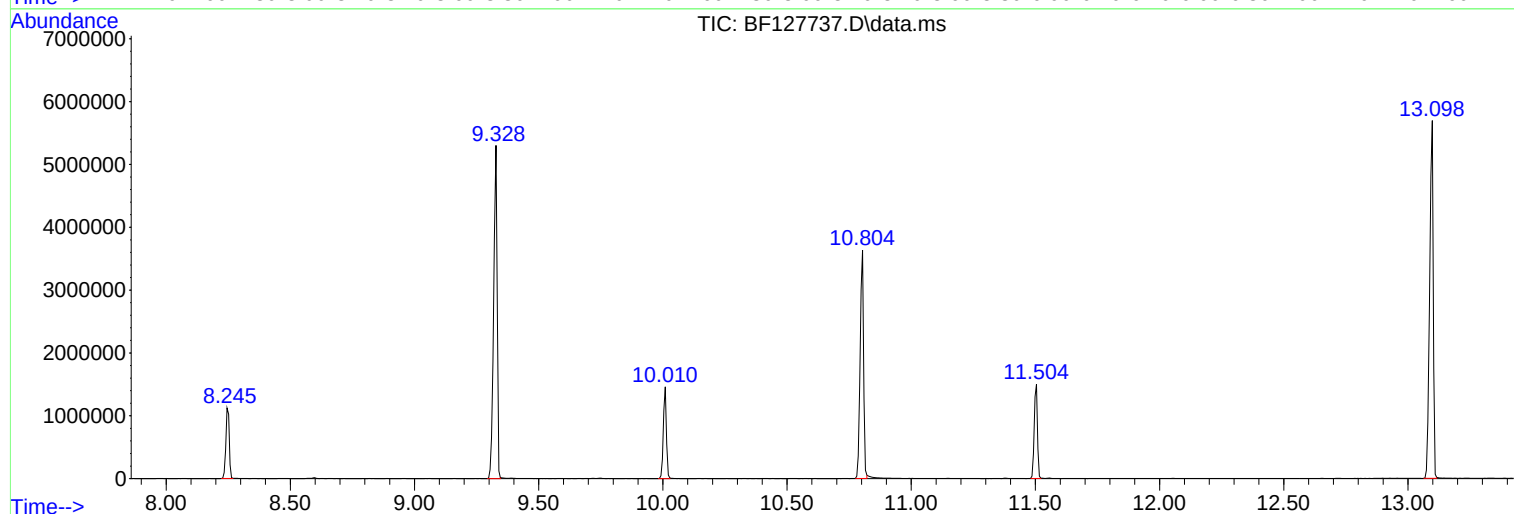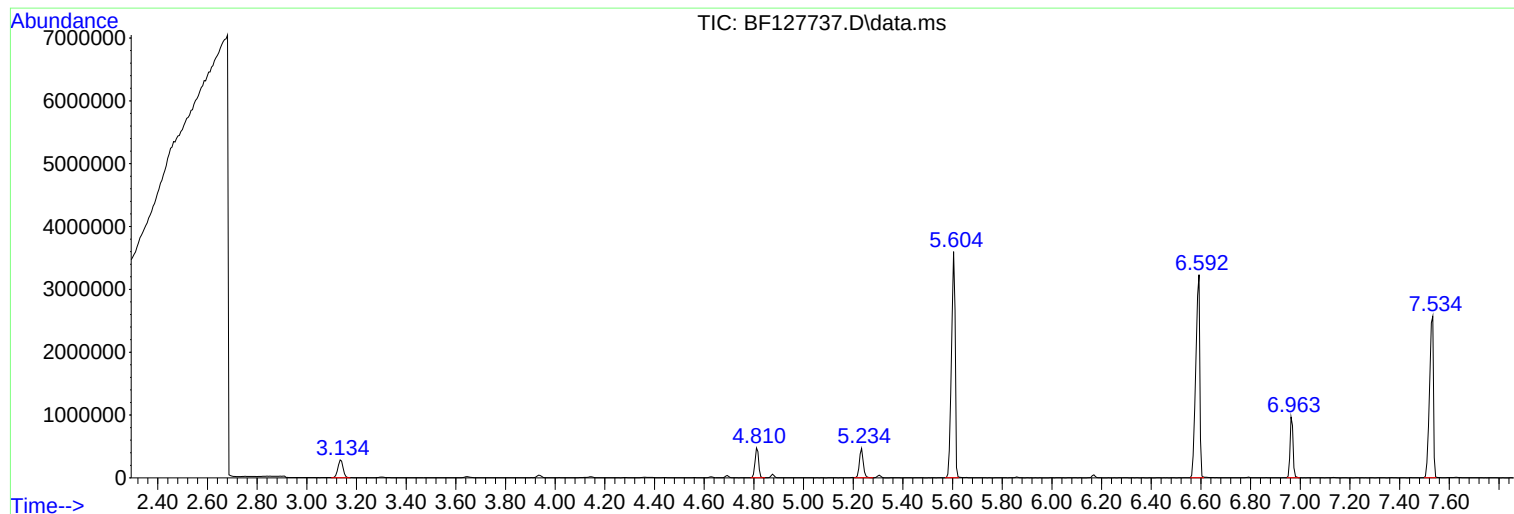

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127737.D
Acq On : 11 Apr 2022 14:30
Operator : CG\JU
Sample : N2335-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A350-CU

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127737.D
Acq On : 11 Apr 2022 14:30
Operator : CG\JU
Sample : N2335-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A350-CU

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------