

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
 Data File : BF127742.D
 Acq On : 11 Apr 2022 16:54
 Operator : CG\JU
 Sample : N2340-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-08-17.5-18.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.587	556	561	564	rBV	2699974	2541803	74.04%	11.894%
2	6.581	725	730	733	rBV	2504184	2635853	76.78%	12.334%
3	6.963	791	795	798	rBV	934920	736191	21.44%	3.445%
4	7.528	885	891	894	rBV	1810557	1753071	51.06%	8.203%
5	8.245	1009	1013	1017	rBV	1098595	945270	27.53%	4.423%
6	9.322	1191	1196	1200	rBV	3287149	3224262	93.91%	15.088%
7	10.010	1309	1313	1316	rBV	1325292	1128776	32.88%	5.282%
8	10.798	1443	1447	1459	rBV	1978001	1741414	50.72%	8.149%
9	11.504	1563	1567	1570	rBV	1412334	1200705	34.97%	5.619%
10	13.092	1833	1837	1840	rBV	3803210	3433186	100.00%	16.065%
11	14.016	1985	1994	2002	rBV3	185899	413880	12.06%	1.937%
12	14.151	2013	2017	2020	rBV	1011581	859619	25.04%	4.023%
13	15.680	2271	2277	2286	rBV	585172	755970	22.02%	3.538%




Sum of corrected areas: 21370000

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127742.D
Acq On : 11 Apr 2022 16:54
Operator : CG\JU
Sample : N2340-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-08-17.5-18.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

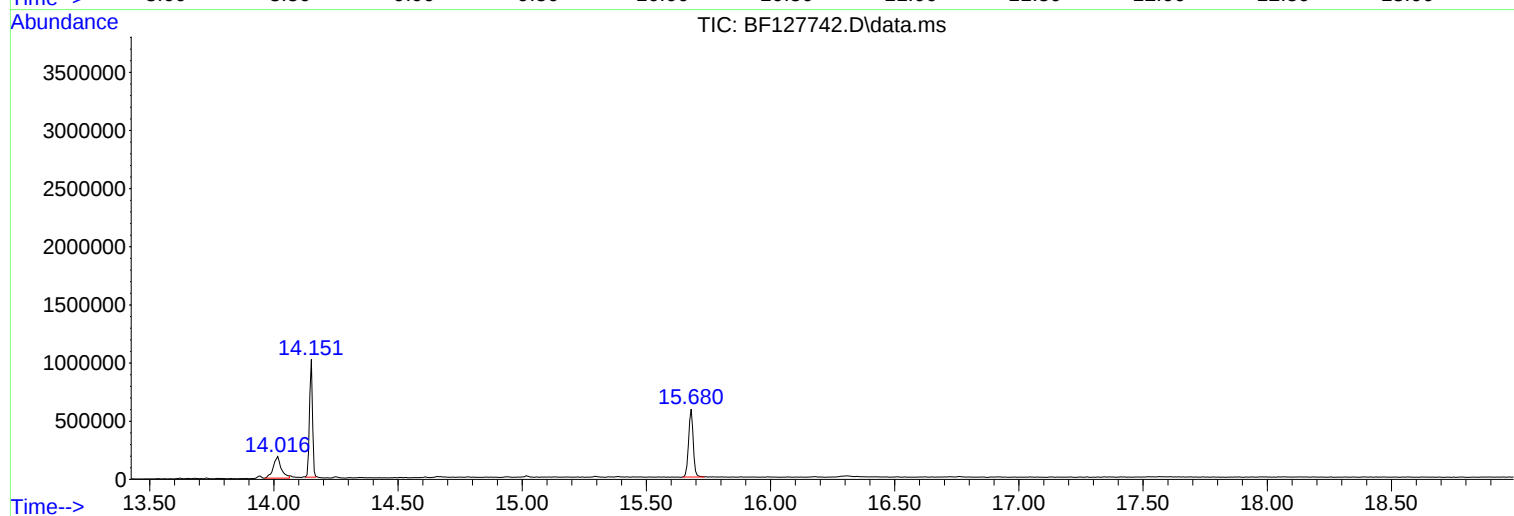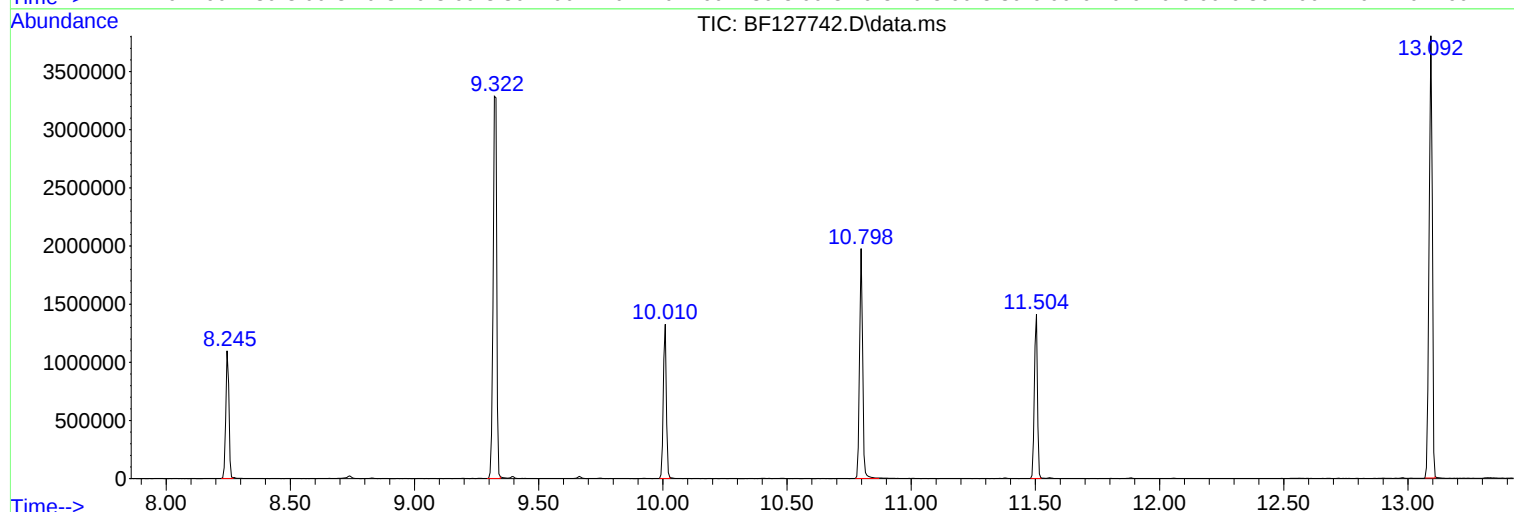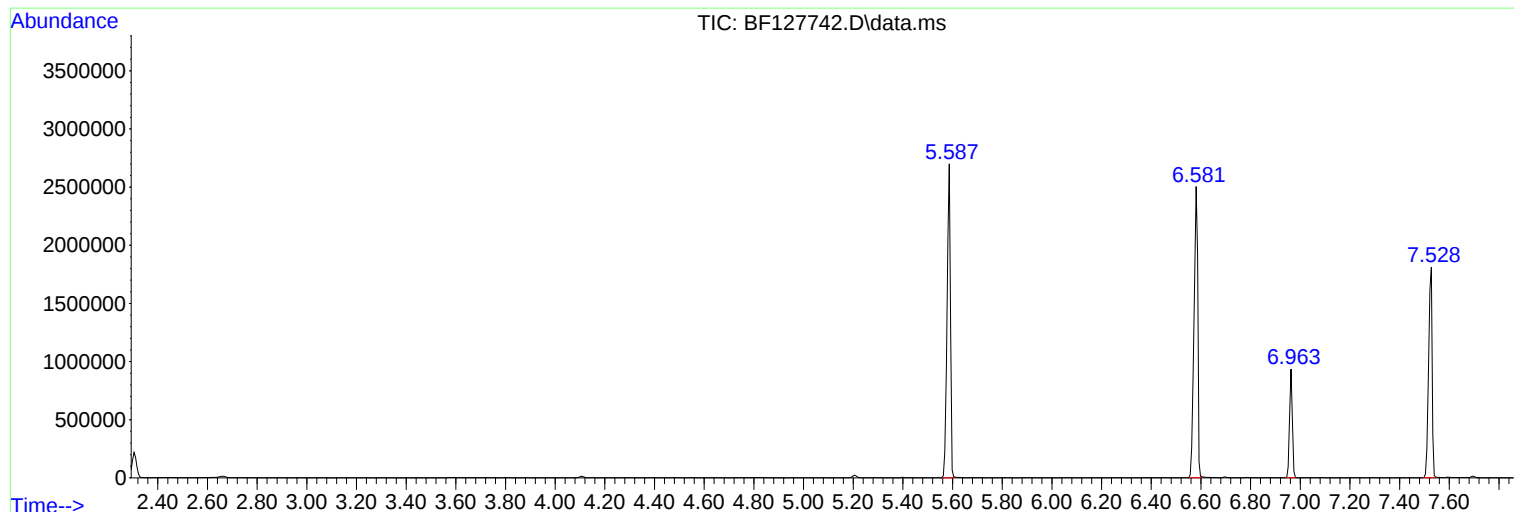

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127742.D
Acq On : 11 Apr 2022 16:54
Operator : CG\JU
Sample : N2340-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-08-17.5-18.0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Octadecanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.015	9.63 ng	413880	Chrysene-d12	14.151

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Octadecanol	270	C18H38O	000112-92-5	50
2			1-Hexadecanol	242	C16H34O	036653-82-4	50
3			1-Tricosene	322	C23H46	018835-32-0	50
4			1-Heneicosanol	312	C21H44O	015594-90-8	45
5			n-Tetracosanol-1	354	C24H50O	000506-51-4	45

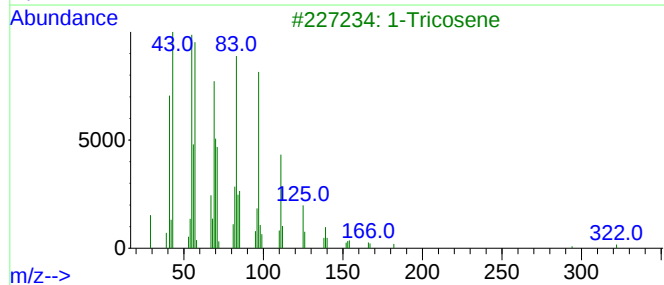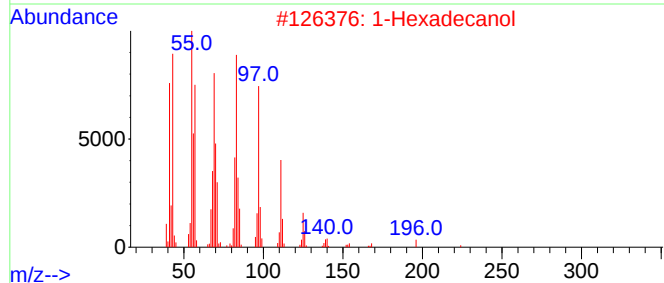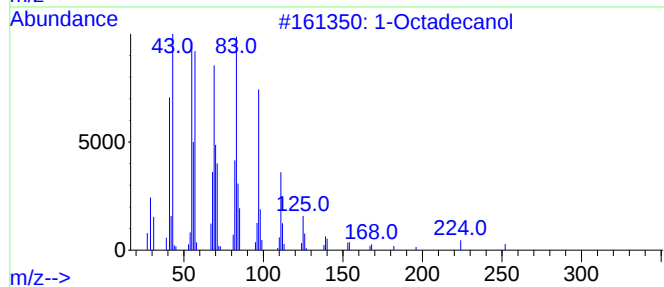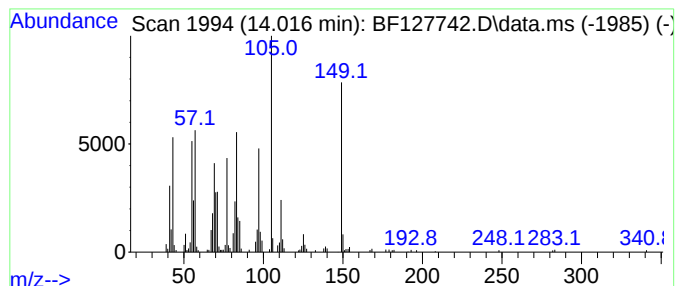

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127742.D
Acq On : 11 Apr 2022 16:54
Operator : CG\JU
Sample : N2340-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-08-17.5-18.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Octadecanol	14.015	9.6	ng	413880	5	14.151	859619	20.0