

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
 Data File : BF127751.D
 Acq On : 11 Apr 2022 21:17
 Operator : CG\JU
 Sample : N2336-02 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 C150-CU

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127751.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.581	555	560	563	rBV	1438475	1242971	75.30%	9.504%
2	6.581	725	730	733	rBV	1638445	1392273	84.35%	10.646%
3	6.963	792	795	799	rBV	948287	834471	50.55%	6.381%
4	7.528	886	891	894	rBV	1112666	938458	56.85%	7.176%
5	8.251	1010	1014	1017	rBV	1325986	1045365	63.33%	7.993%
6	9.328	1193	1197	1200	rBV	1978164	1650622	100.00%	12.622%
7	10.010	1309	1313	1317	rBV	1269866	1080158	65.44%	8.259%
8	10.039	1317	1318	1322	rVB	23177	20241	1.23%	0.155%
9	10.216	1342	1348	1351	rBV2	20066	35209	2.13%	0.269%
10	10.557	1403	1406	1411	rVB	25769	25459	1.54%	0.195%
11	10.716	1431	1433	1438	rVB2	18314	19144	1.16%	0.146%
12	10.798	1444	1447	1453	rBV	771893	672632	40.75%	5.143%
13	11.045	1486	1489	1494	rBV7	17603	32799	1.99%	0.251%
14	11.151	1505	1507	1512	rBV6	21939	24019	1.46%	0.184%
15	11.504	1563	1567	1569	rBV	1044268	867870	52.58%	6.636%
16	11.527	1569	1571	1575	rVB	340054	248559	15.06%	1.901%
17	11.580	1577	1580	1583	rVV	51507	41767	2.53%	0.319%
18	12.016	1651	1654	1656	rBV3	67310	76780	4.65%	0.587%
19	12.721	1771	1774	1777	rBV	359921	284708	17.25%	2.177%
20	12.951	1811	1813	1818	rVB	274368	228378	13.84%	1.746%
21	13.092	1834	1837	1840	rBV	1311155	1019313	61.75%	7.794%
22	14.157	2014	2018	2020	rBV	774595	781117	47.32%	5.973%
23	15.686	2275	2278	2287	rVB	377913	515468	31.23%	3.942%




Sum of corrected areas: 13077781

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127751.D
Acq On : 11 Apr 2022 21:17
Operator : CG\JU
Sample : N2336-02 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C150-CU

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

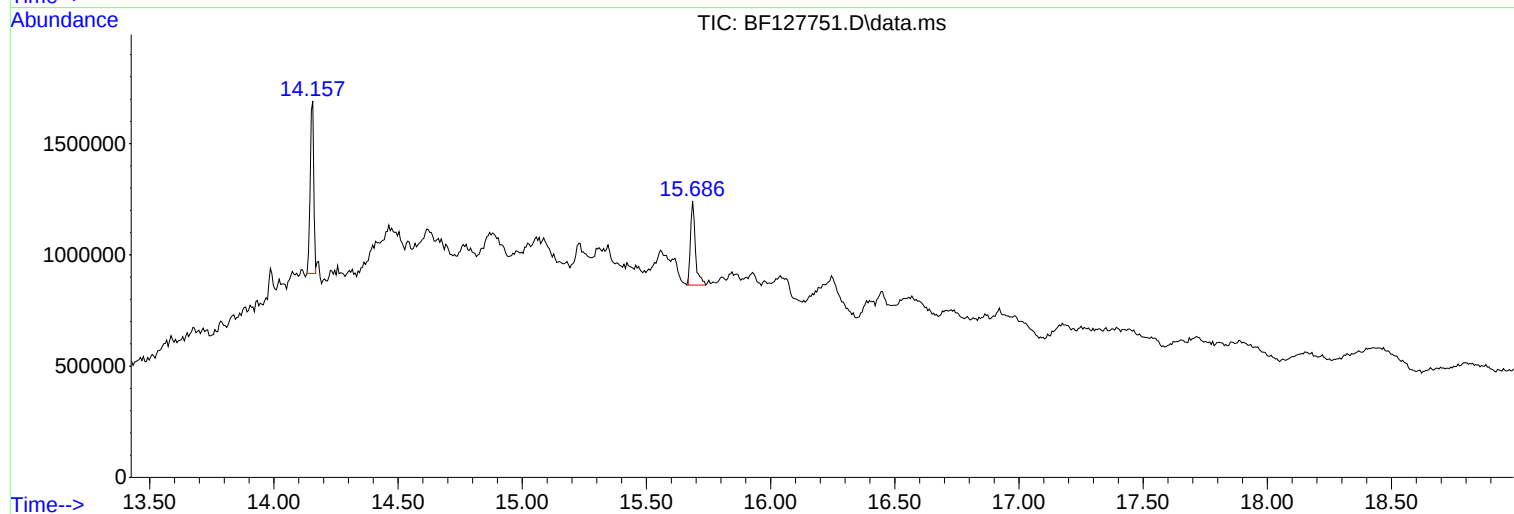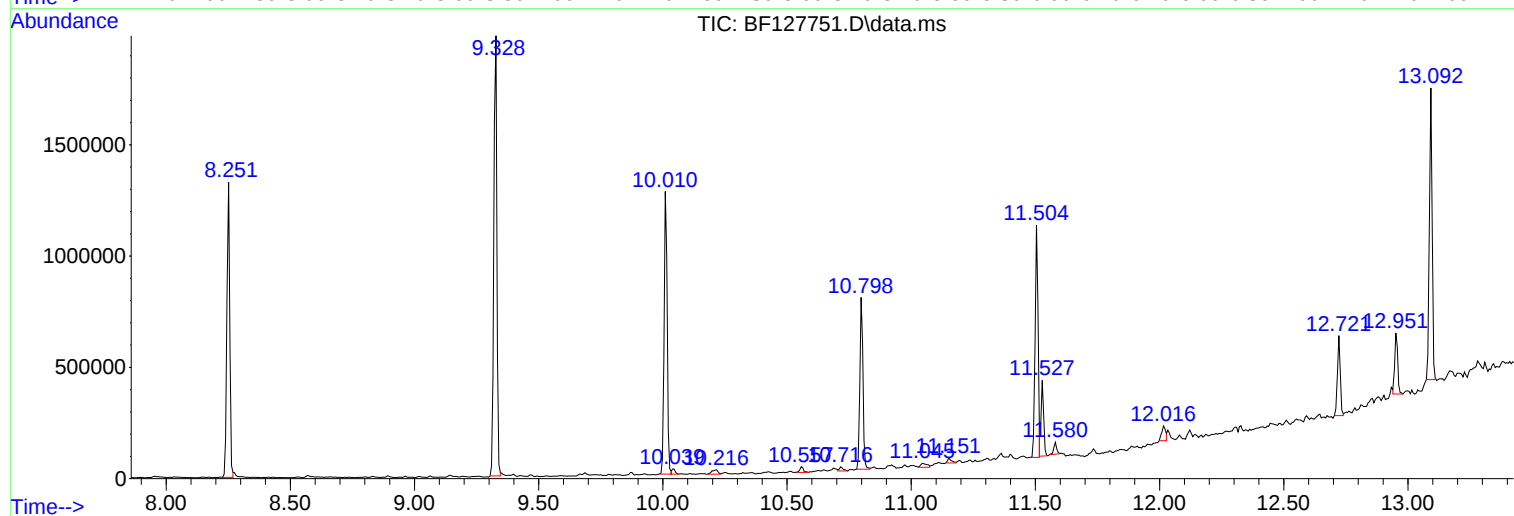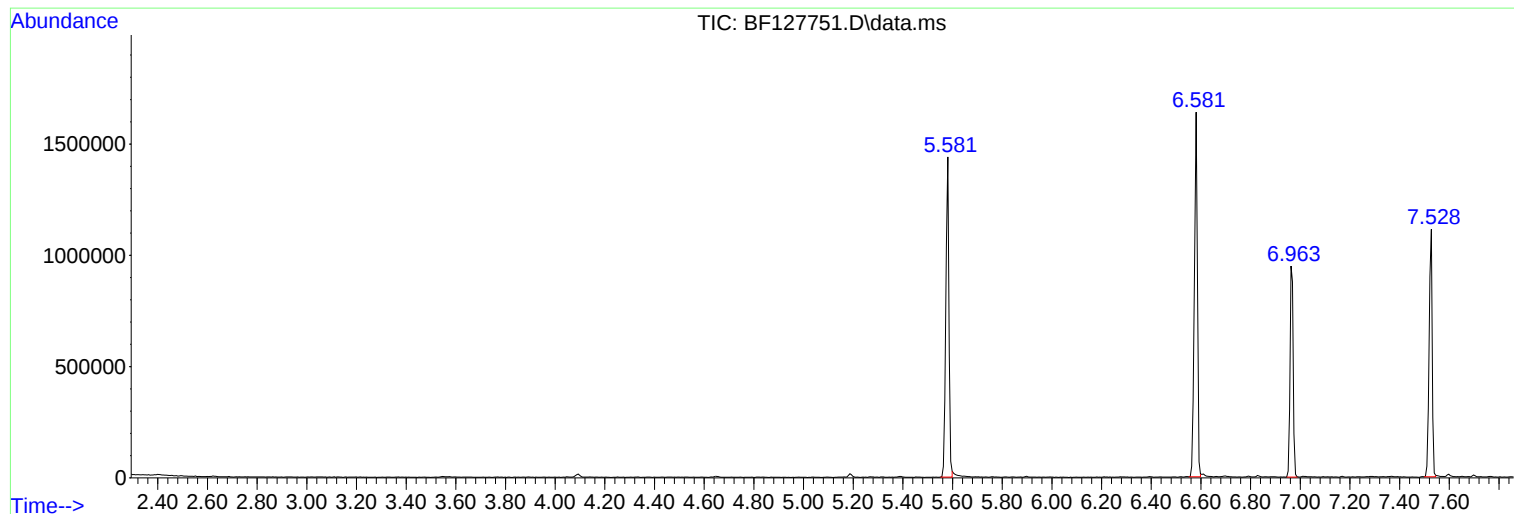

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127751.D
Acq On : 11 Apr 2022 21:17
Operator : CG\JU
Sample : N2336-02 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C150-CU

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041122\
Data File : BF127751.D
Acq On : 11 Apr 2022 21:17
Operator : CG\JU
Sample : N2336-02 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C150-CU

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------