
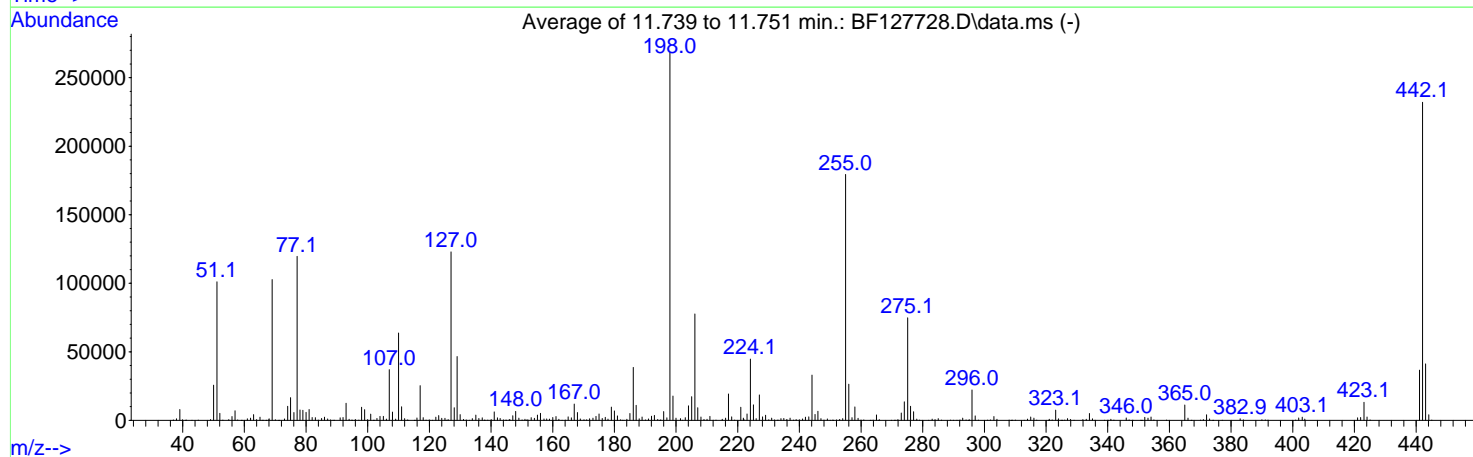


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041122\  
 Data File : BF127728.D  
 Acq On : 11 Apr 2022 09:32  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Apr 06 13:55:27 2022

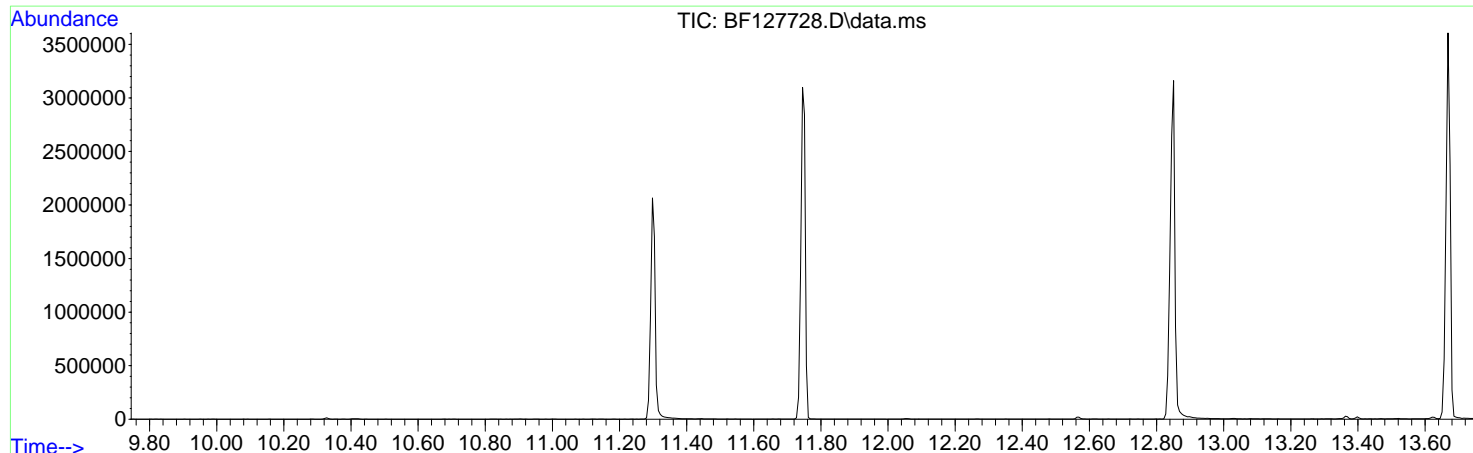




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	101077	PASS
68	69	0.00	2	1.2	1209	PASS
69	198	0.00	100	38.3	102680	PASS
70	69	0.00	2	0.5	496	PASS
127	198	10	80	45.8	122885	PASS
197	198	0.00	2	0.7	1915	PASS
198	198	100	100	100.0	268373	PASS
199	198	5	9	6.6	17767	PASS
275	198	10	60	27.9	74872	PASS
365	198	1	100	4.2	11256	PASS
441	198	0.01	100	13.7	36636	PASS
442	442	50	100	100.0	232088	PASS
443	442	15	24	17.8	41276	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041122\  
 Data File : BF127728.D  
 Acq On : 11 Apr 2022 09:32  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 11 18:58:57 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Apr 06 13:55:27 2022  
 Response via : Initial Calibration

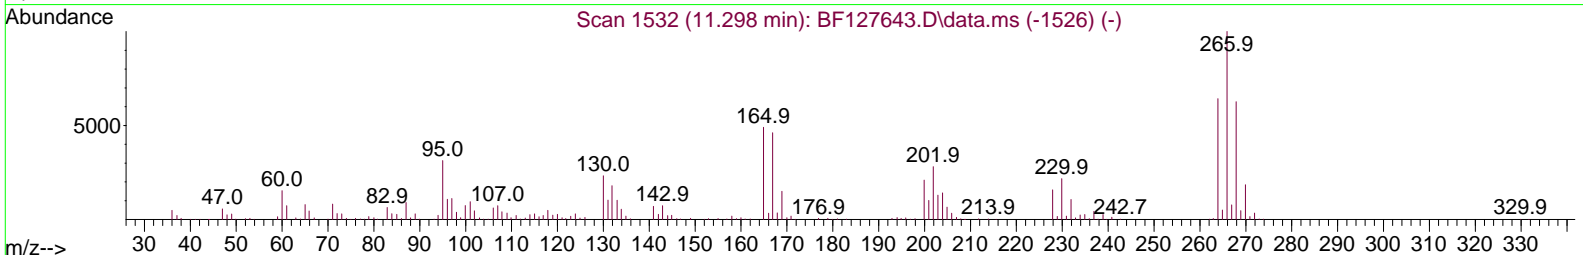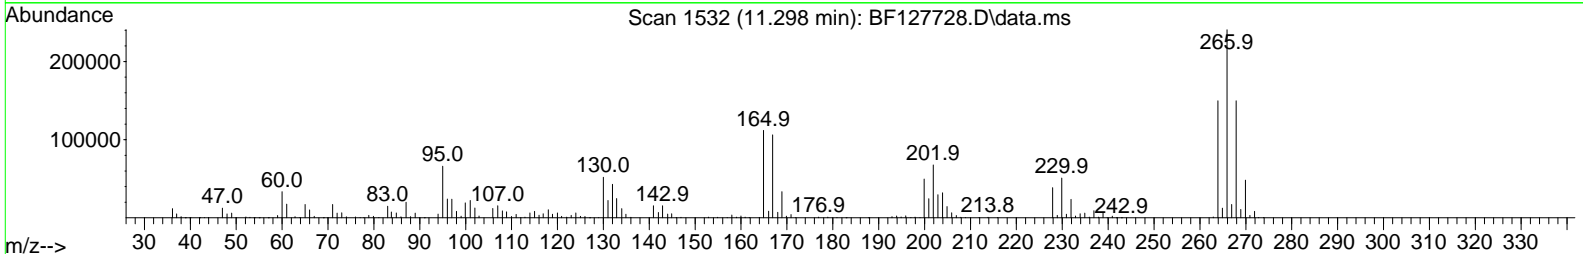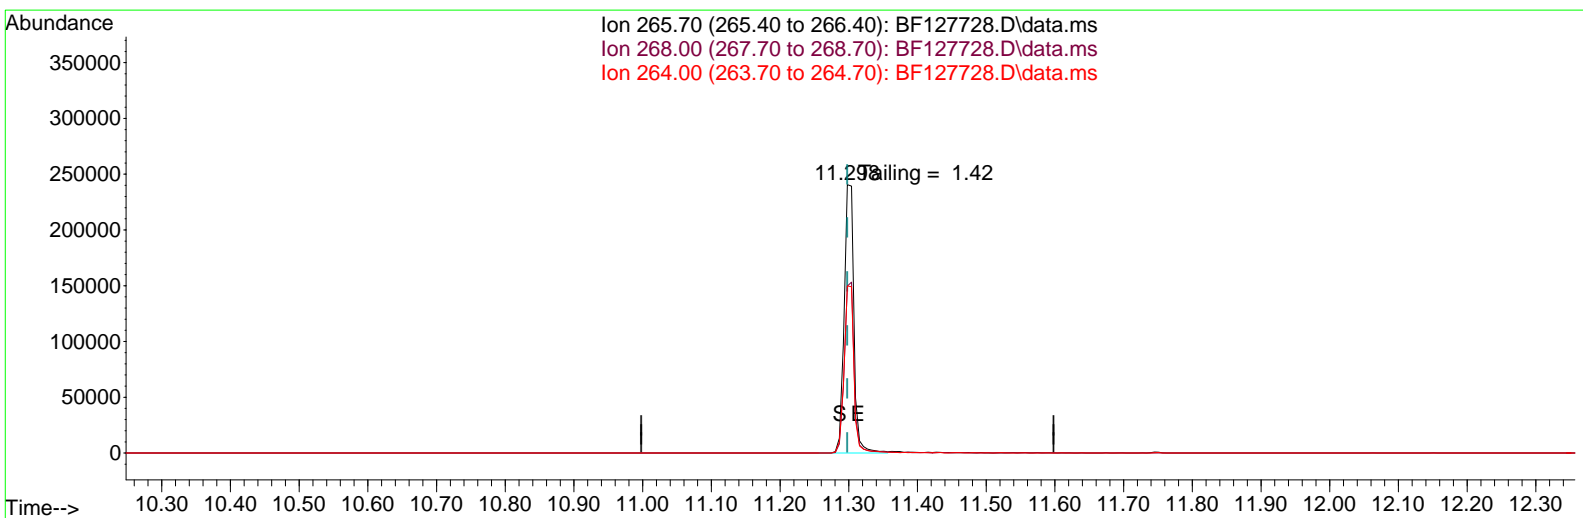

TIC: BF127728.D\data.ms

(70) Pentachlorophenol (C)




11.298min (-0.000) 393219.19 ng

response	236797	
Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.21
264.00	60.60	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041122\  
 Data File : BF127728.D  
 Acq On : 11 Apr 2022 09:32  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 11 18:58:57 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Apr 06 13:55:27 2022  
 Response via : Initial Calibration

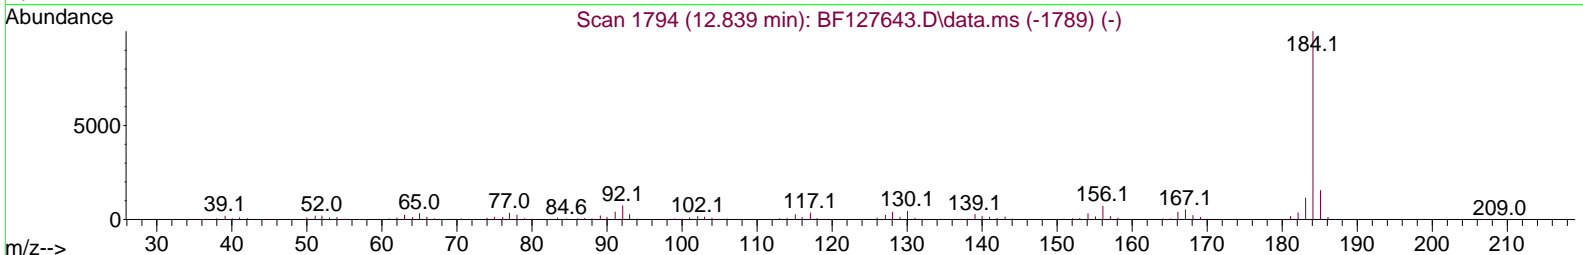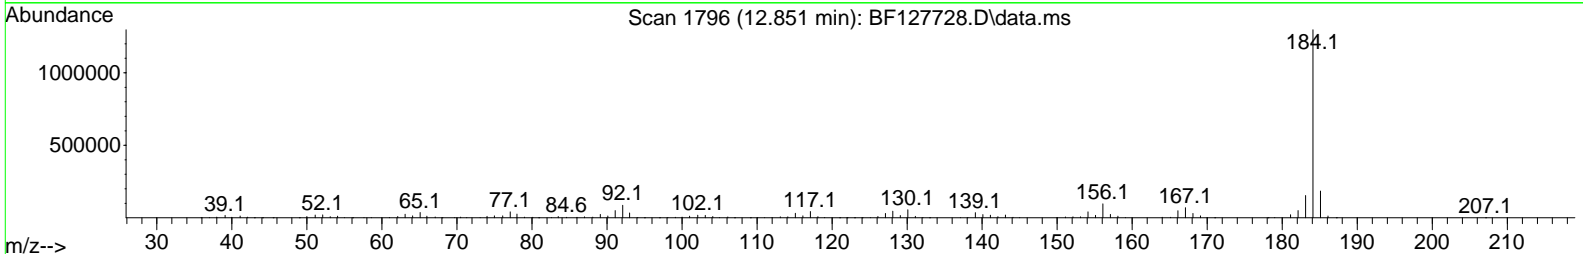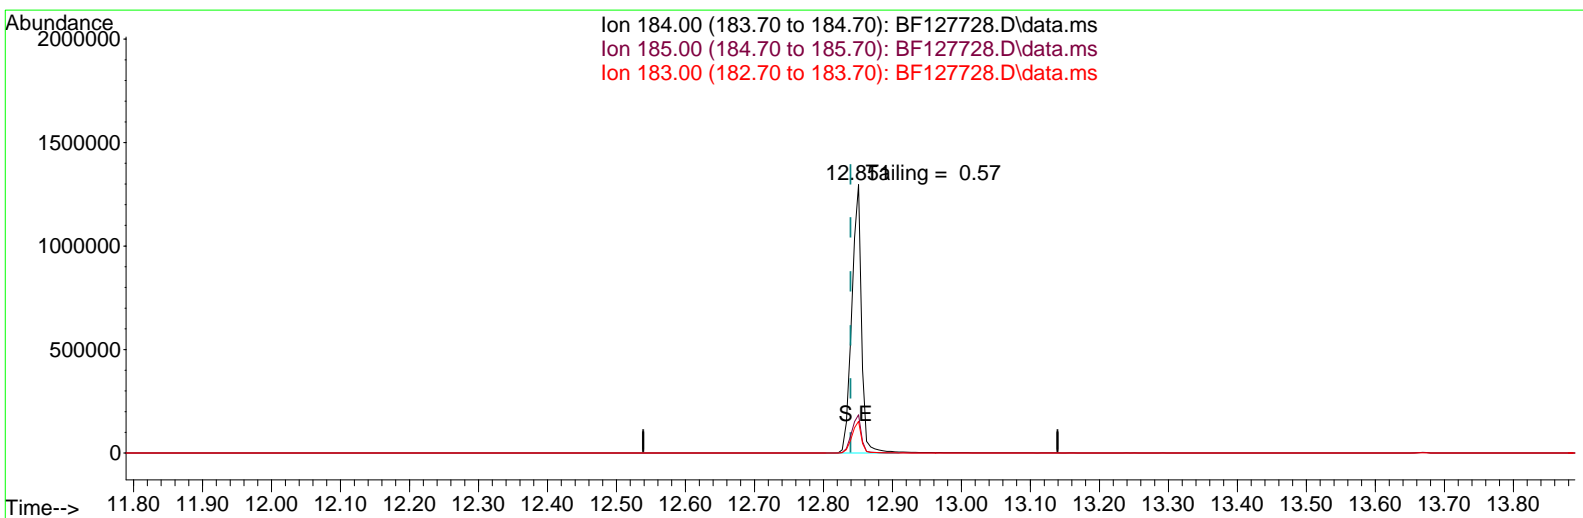

TIC: BF127728.D\data.ms

(77) Benzidine

12.851min (+ 0.012) 5973.84 ng m

response 1257194

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.25
183.00	11.70	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/11/2022	BNA_F	<u>BF127728.D</u>
Compound Name	Response	Retention Time
DDT	577637	13.66
DDD	4436	13.36
DDE	583	13.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5019	582656	0.86

Instrument :  
 BNA\_F  
 ClientSampled :  
 DFTPP