


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041123\
Data File : BF132844.D
Acq On : 11 Apr 2023 11:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 12 03:34:19 2023

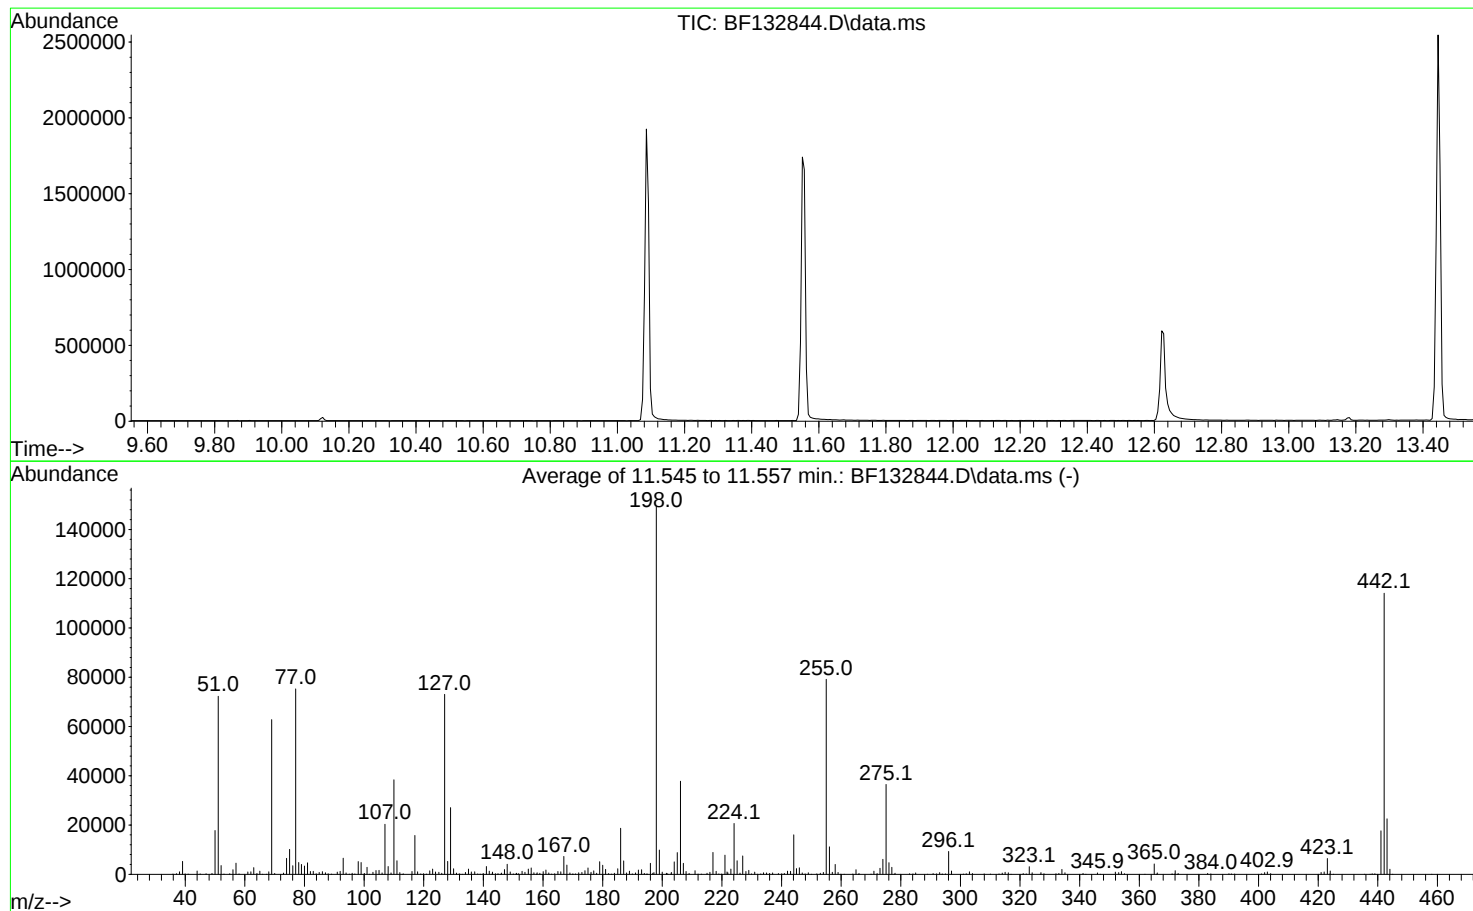

AutoFind: Scans 1523, 1524, 1525; Background Corrected with Scan 1518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	72251	PASS
68	69	0.00	2	1.6	999	PASS
69	198	0.00	100	42.1	62811	PASS
70	69	0.00	2	0.6	376	PASS
127	198	10	80	48.9	73048	PASS
197	198	0.00	2	0.4	671	PASS
198	198	100	100	100.0	149363	PASS
199	198	5	9	6.6	9838	PASS
275	198	10	60	24.4	36451	PASS
365	198	1	100	2.8	4165	PASS
441	198	0.01	100	11.8	17614	PASS
442	442	50	100	100.0	114092	PASS
443	442	15	24	19.7	22492	PASS